

Sample Name :VIP, human, ovine, porcine, rat
 Cat No. :RP10085
 Lot No. :PE5481902
 Time Processed :23:40:15
 Month-Day-Year Processed :02/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Pumps | Solvent B Conc. | 5 |
| 33.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

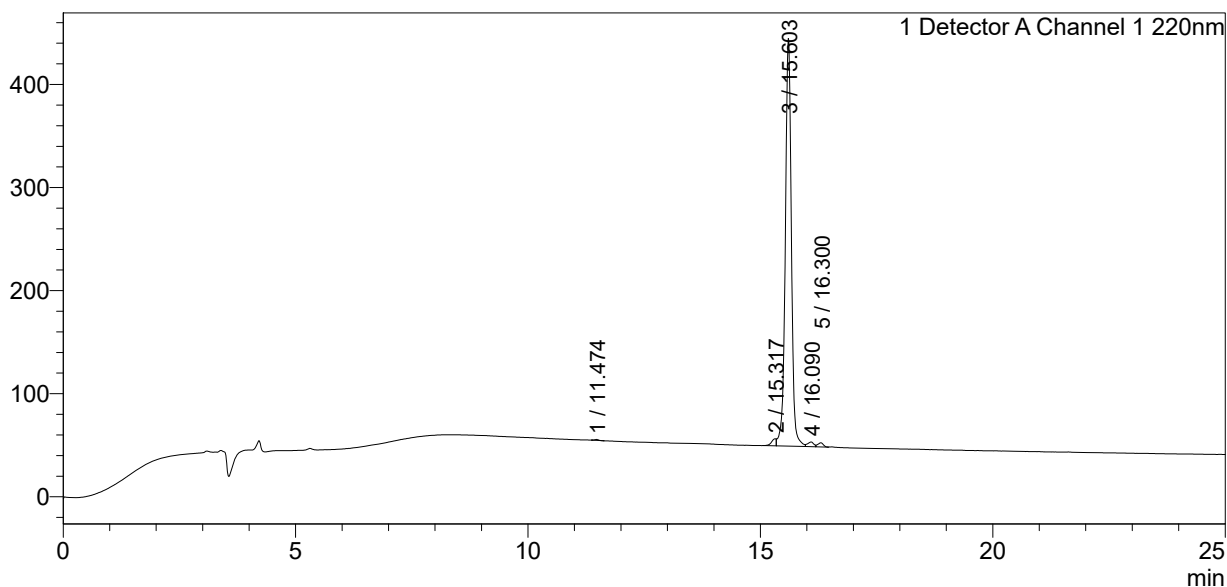

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 11.474 | 5158 | 897 | 0.140 |
| 2 | 15.317 | 47581 | 6839 | 1.287 |
| 3 | 15.603 | 3569660 | 395408 | 96.582 |
| 4 | 16.090 | 41675 | 4581 | 1.128 |
| 5 | 16.300 | 31910 | 3958 | 0.863 |
| Total | | 3695983 | 411682 | 100.000 |