

Sample Name :Bradykinin
 Cat No. :RP11129
 Lot No. :E7876221F
 Time Processed :4:43:14 AM
 Month-Day-Year Processed :07/06/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

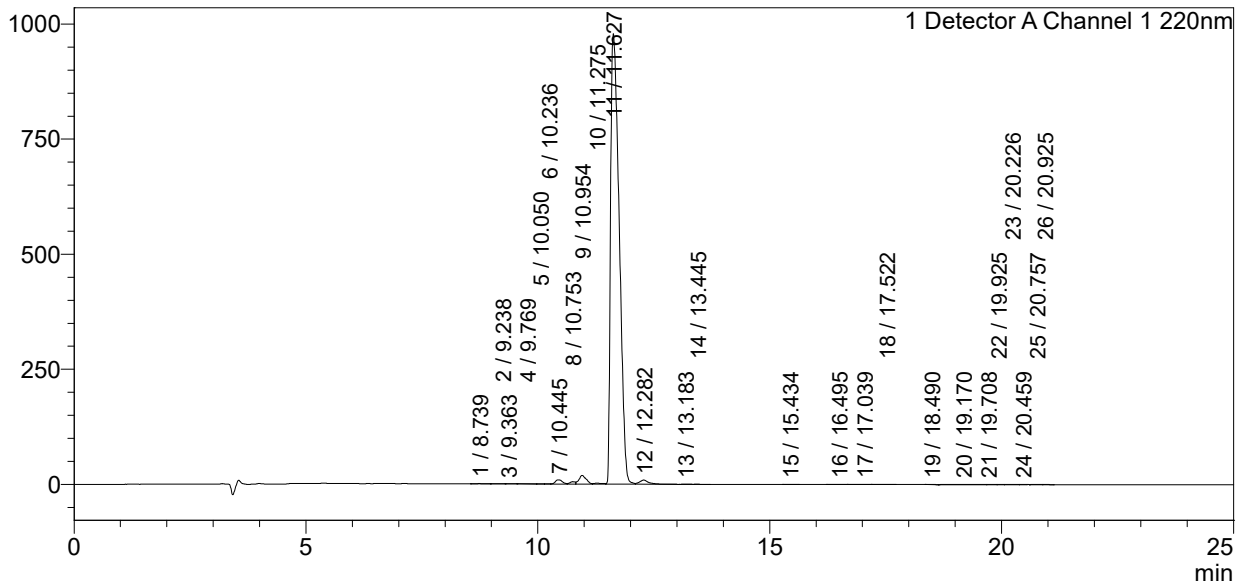

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.739	5027	657	0.038
2	9.238	2095	197	0.016
3	9.363	2155	209	0.016
4	9.769	8696	530	0.066
5	10.050	2770	317	0.021
6	10.236	3561	570	0.027
7	10.445	97006	9192	0.736
8	10.753	40800	5144	0.310
9	10.954	203033	18943	1.541
10	11.275	26491	2109	0.201
11	11.627	12595456	979083	95.577
12	12.282	130080	9107	0.987
13	13.183	2622	255	0.020
14	13.445	2021	178	0.015

Peak#	Ret. Time	Area	Height	Area%
15	15.434	1359	116	0.010
16	16.495	3193	196	0.024
17	17.039	7319	417	0.056
18	17.522	4943	260	0.038
19	18.490	1156	149	0.009
20	19.170	25090	677	0.190
21	19.708	3190	284	0.024
22	19.925	1755	218	0.013
23	20.226	2866	191	0.022
24	20.459	1029	128	0.008
25	20.757	3505	332	0.027
26	20.925	1086	148	0.008
Total		13178303	1029610	100.000