


Mass Spectrum

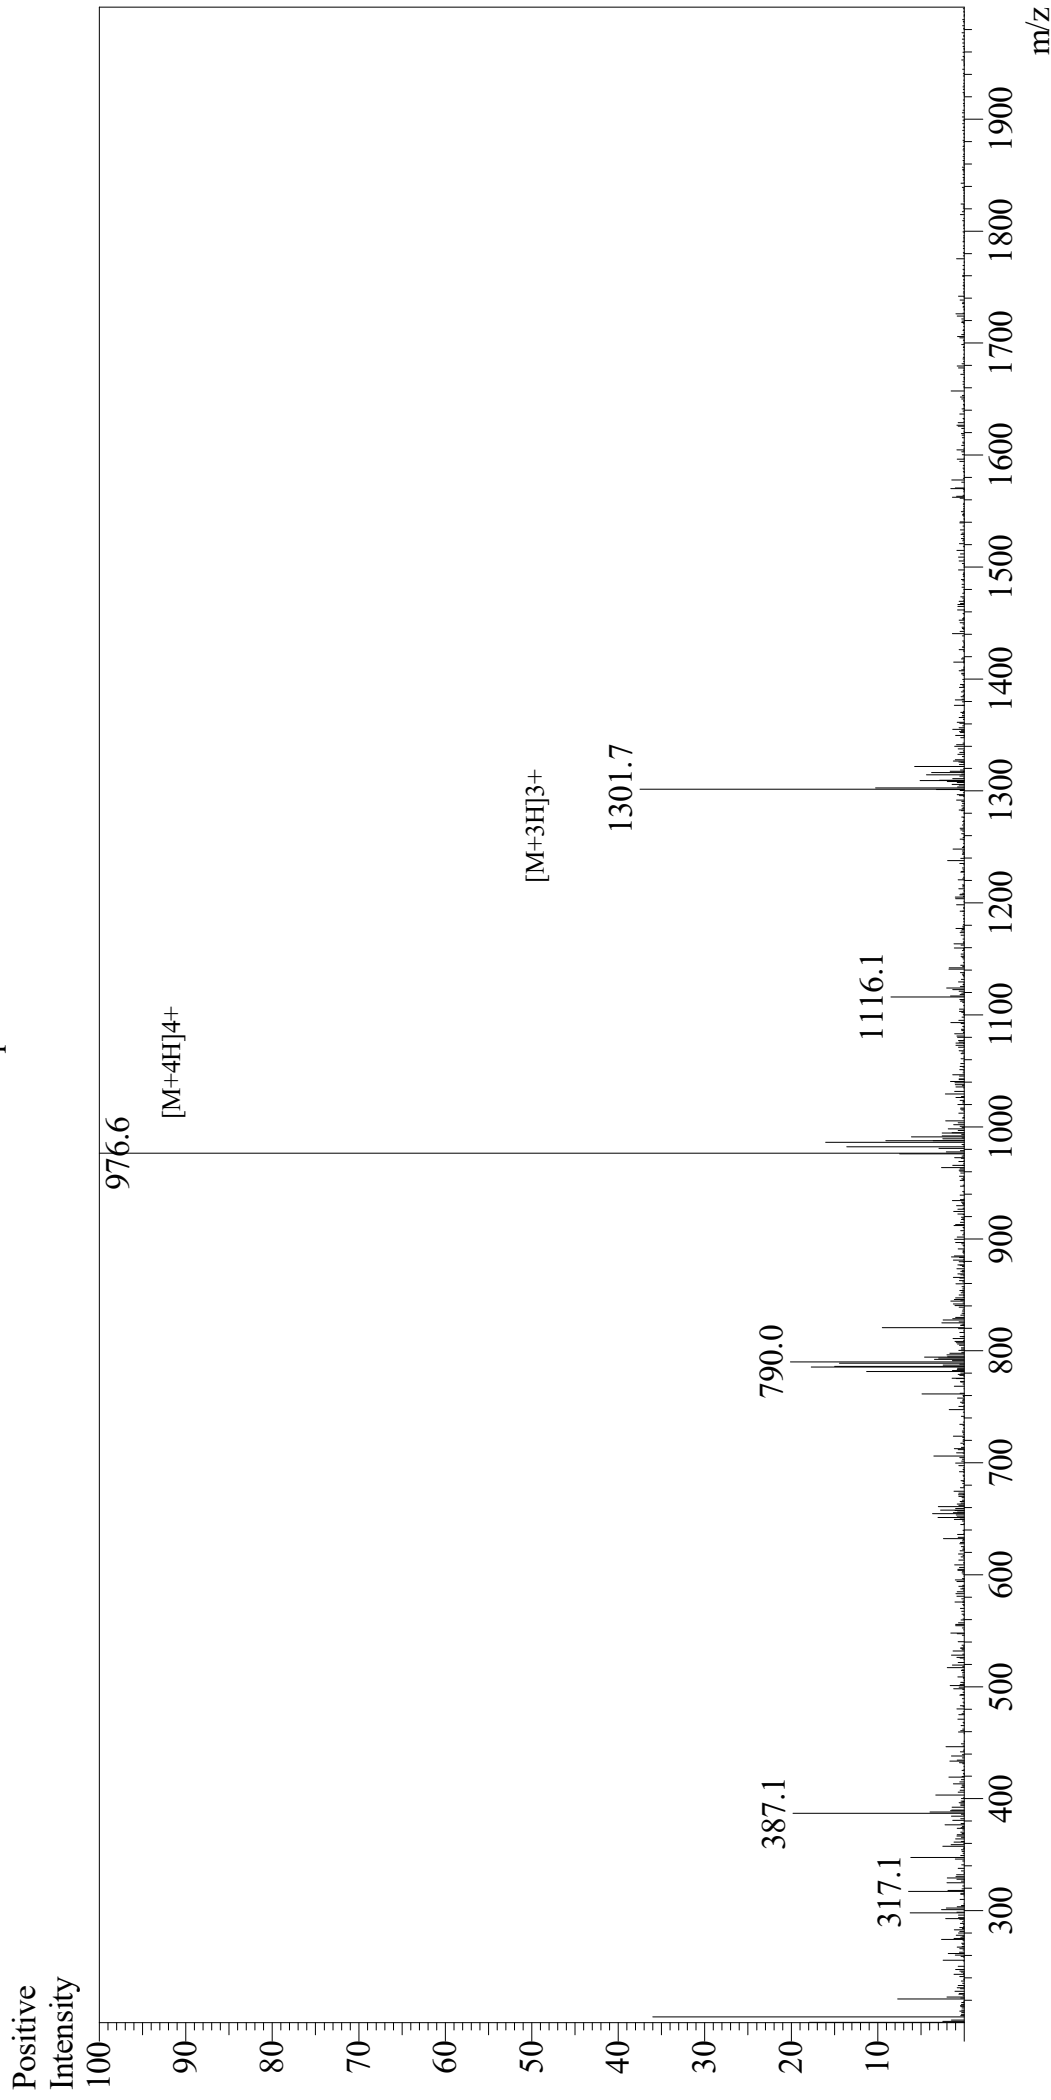

Sample Information

User : Gary
Month-Day Processed : 02/19/20
Time Processed : 03:54:51 PM
Injection Volume : 0.3
Sample Name : Amylin, human, amide
Cat No. : RP11278
Lot No. : E6382620B
Theoretical MW : 3903.28
Observed MW : 3902.4

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH