

Sample Name :DYKDDDDK Peptide  
 Cat No.: RP10586  
 Lot No.: E7993420I  
 Time Processed :8:18:43  
 Month-Day-Year Processed :10/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

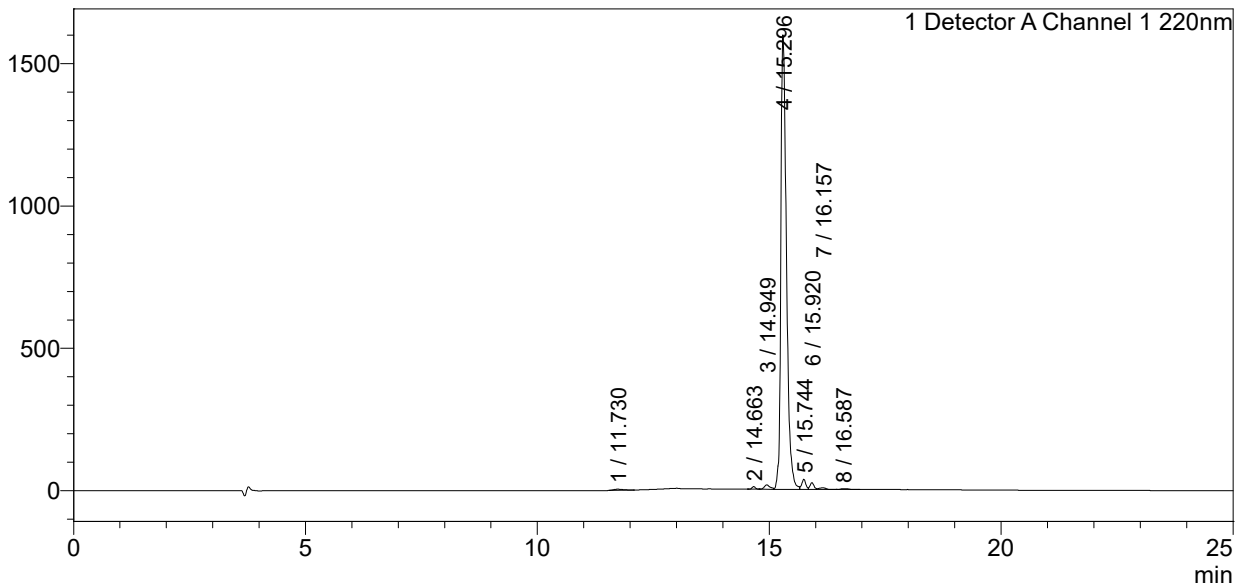

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.730	53884	3736	0.381
2	14.663	48117	9243	0.340
3	14.949	134740	15508	0.953
4	15.296	13469152	1596837	95.288
5	15.744	212572	35419	1.504
6	15.920	135257	23509	0.957
7	16.157	56575	5638	0.400
8	16.587	24871	2250	0.176
Total		14135170	1692138	100.000