

Sample Name:Angiotensin II, human  
 Cat. No. : RP11257  
 Lot. No. : E4906720K  
 Time Processed :12:52:09 PM  
 Month-Day-Year Processed :11/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

mV

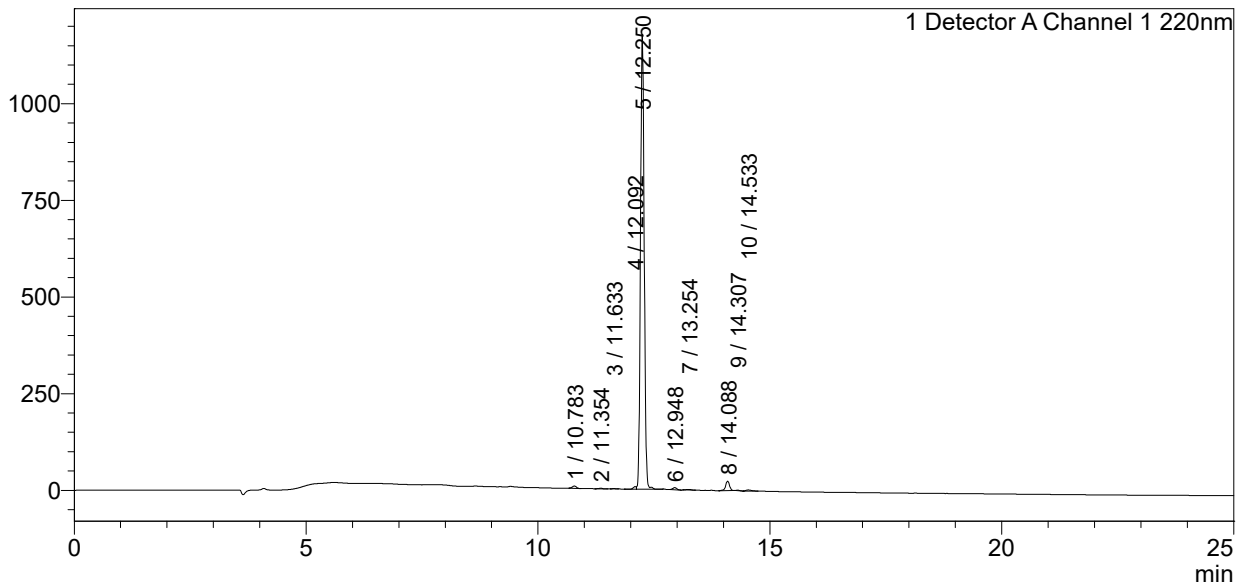

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.783	39077	6224	0.575
2	11.354	7894	1561	0.116
3	11.633	1292	377	0.019
4	12.092	31242	6683	0.460
5	12.250	6502575	1176096	95.648
6	12.948	29158	5145	0.429
7	13.254	13781	1757	0.203
8	14.088	145626	24547	2.142
9	14.307	5404	1390	0.079
10	14.533	22423	2783	0.330
Total		6798472	1226564	100.000