

Sample Name : (Arg)9
 Cat. No. : RP20403
 Lot. No. : PE8851902
 Time Processed : 5:48:21
 Month-Day-Year Processed : 03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment : SS-CM-0310

Chromatogram

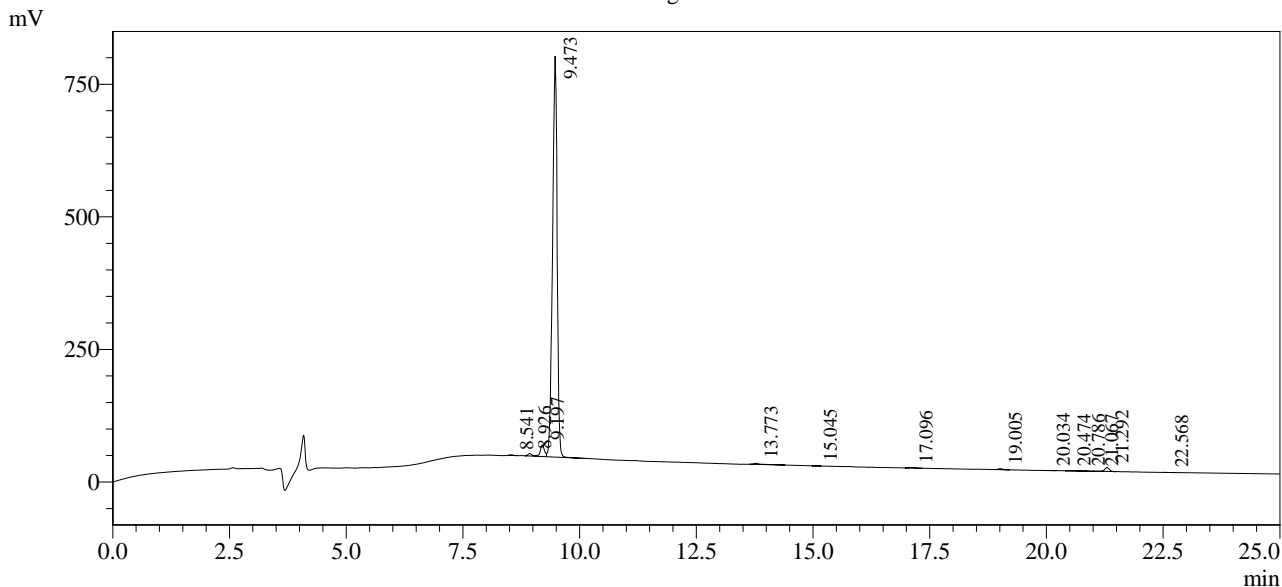

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.541	4942	1099	0.090
2	8.926	25702	4527	0.470
3	9.197	137240	22091	2.511
4	9.473	5192685	755851	95.015
5	13.773	25962	2155	0.475
6	15.045	2597	474	0.048
7	17.096	6978	842	0.128
8	19.005	12227	1878	0.224
9	20.034	1920	227	0.035
10	20.474	2514	235	0.046
11	20.786	2222	260	0.041
12	21.067	1006	180	0.018
13	21.292	47982	7368	0.878
14	22.568	1128	220	0.021
Total		5465104	797407	100.000