

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : PE1601611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

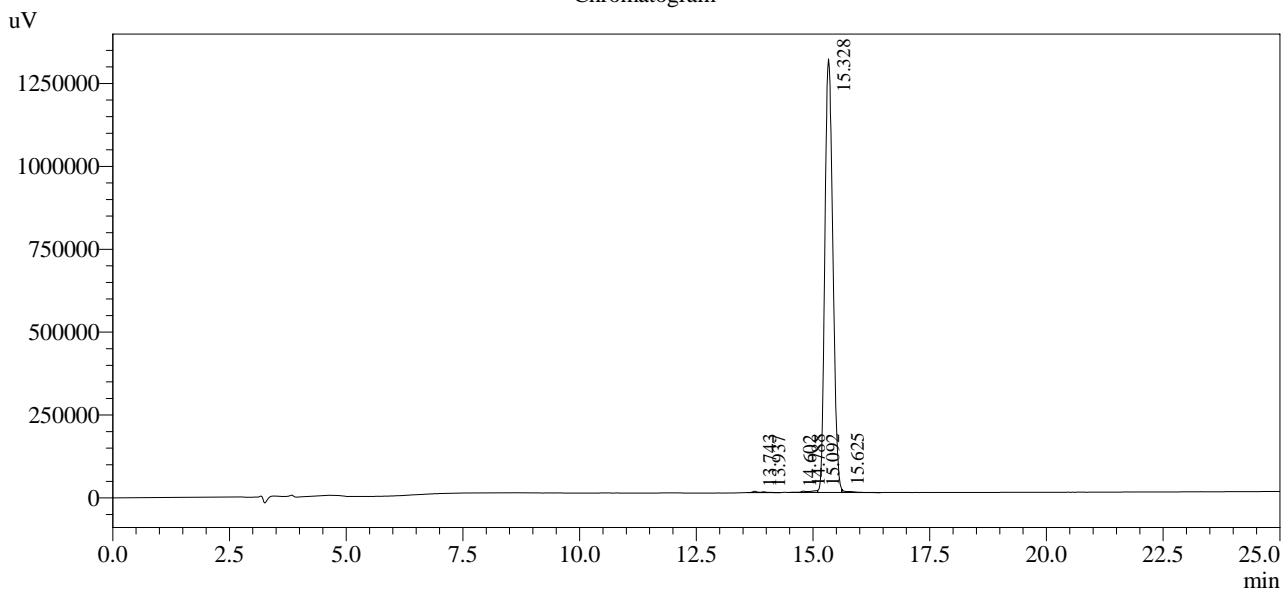

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.743	29790	4104	0.188
2	13.937	24668	2535	0.156
3	14.602	4363	492	0.028
4	14.788	28385	4152	0.179
5	15.092	58409	5981	0.369
6	15.328	15612902	1308148	98.646
7	15.625	68716	8217	0.434
Total		15827233	1333629	100.000