

Sample Name :Neuropeptide Y (13-36), human
 Cat. No. :RP10488
 Lot. No. :PE6861811
 Time Processed :9:21:43
 Month-Day-Year Processed :11/30/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|--------------|-------|---------|
| 0.01 | Pumps | Pump B Conc. | 5 | |
| 25.00 | Pumps | Pump B Conc. | 65 | |
| 25.01 | Pumps | Pump B Conc. | 95 | |
| 27.00 | Pumps | Pump B Conc. | 95 | |
| 27.01 | Pumps | Pump B Conc. | 5 | |
| 35.00 | Pumps | Pump B Conc. | 5 | |
| 35.01 | Controller | Stop | | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

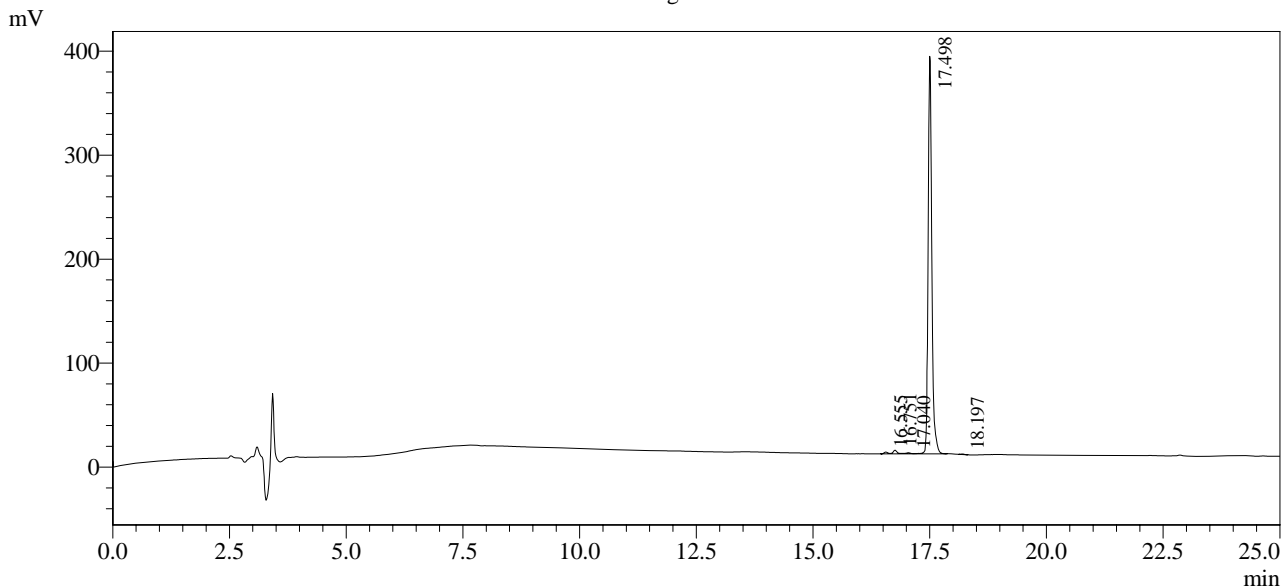

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 16.555 | 10438 | 1797 | 0.487 |
| 2 | 16.751 | 22396 | 3535 | 1.045 |
| 3 | 17.040 | 8154 | 1067 | 0.381 |
| 4 | 17.498 | 2098592 | 382434 | 97.966 |
| 5 | 18.197 | 2574 | 553 | 0.120 |
| Total | | 2142154 | 389387 | 100.000 |