

Sample Name :DYKDDDDK Peptide  
 Cat No.: RP10586  
 Lot No.: E3534820I  
 Time Processed :14:27:09  
 Month-Day-Year Processed :10/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

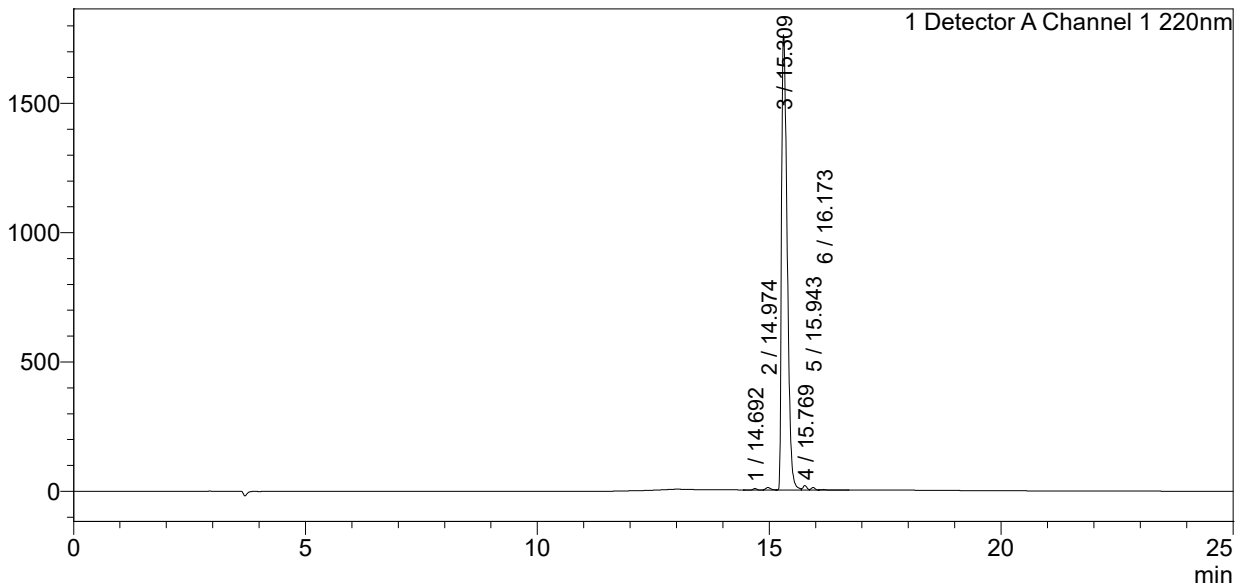

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.692	29582	5897	0.194
2	14.974	71258	9737	0.466
3	15.309	15006737	1760677	98.184
4	15.769	104088	17875	0.681
5	15.943	58053	10264	0.380
6	16.173	14658	2050	0.096
Total		15284376	1806499	100.000