

Sample Name :Angiotensin II (1-4), human
 Cat No. :RP11252
 Lot No. :E2124521A
 Time Processed :10:52:51 AM
 Month-Day-Year Processed :01/10/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

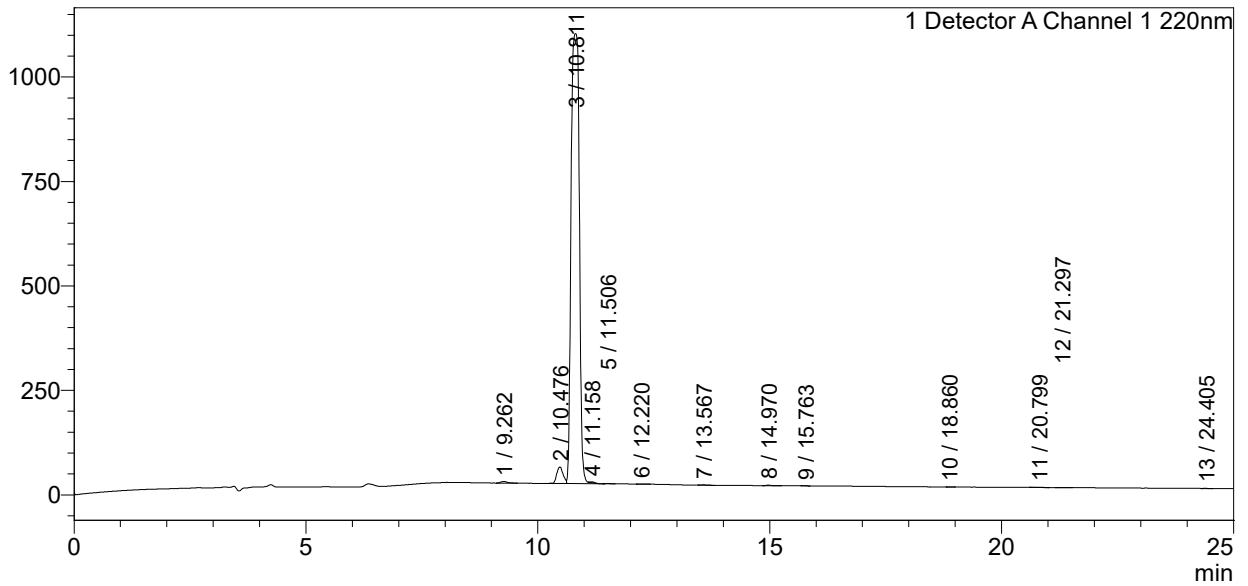

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.262	33867	3666	0.248
2	10.476	377842	39675	2.765
3	10.811	13206145	1077176	96.641
4	11.158	13415	2079	0.098
5	11.506	4863	700	0.036
6	12.220	3292	406	0.024
7	13.567	5846	696	0.043
8	14.970	9045	1142	0.066
9	15.763	1395	243	0.010
10	18.860	1007	194	0.007
11	20.799	5023	460	0.037
12	21.297	2302	194	0.017
13	24.405	1062	178	0.008
Total		13665103	1126809	100.000