

Sample Name : Fibronectin CS1 Peptide
 Cat. No. : RP10838
 Lot. No. : PE4871611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

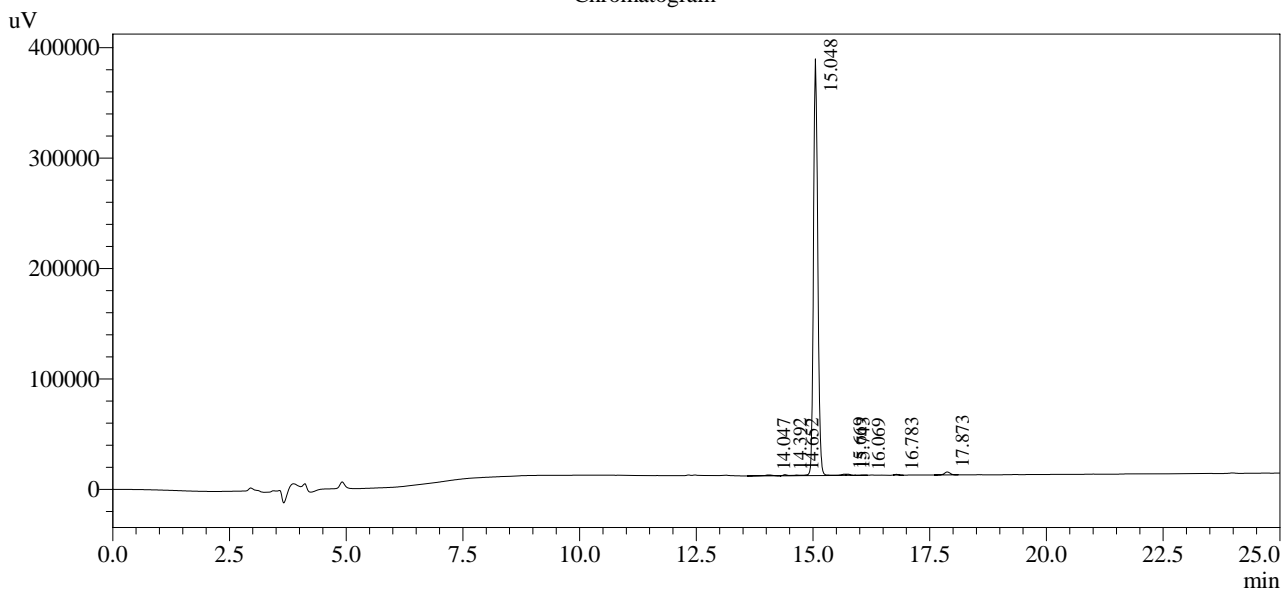

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.047	12073	863	0.484
2	14.392	6859	1034	0.275
3	14.652	5813	589	0.233
4	15.048	2429121	377291	97.334
5	15.669	8106	1076	0.325
6	15.743	5690	1061	0.228
7	16.069	315	53	0.013
8	16.783	3600	647	0.144
9	17.873	24079	2706	0.965
Total		2495657	385321	100.000