

Sample Name : Fibronectin CS1 Peptide
 Cat. No. : RP10838
 Lot. No. : E8084021C
 Time Processed: 14:52:46
 Year-Month-Day: 2021/3/10

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 <<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

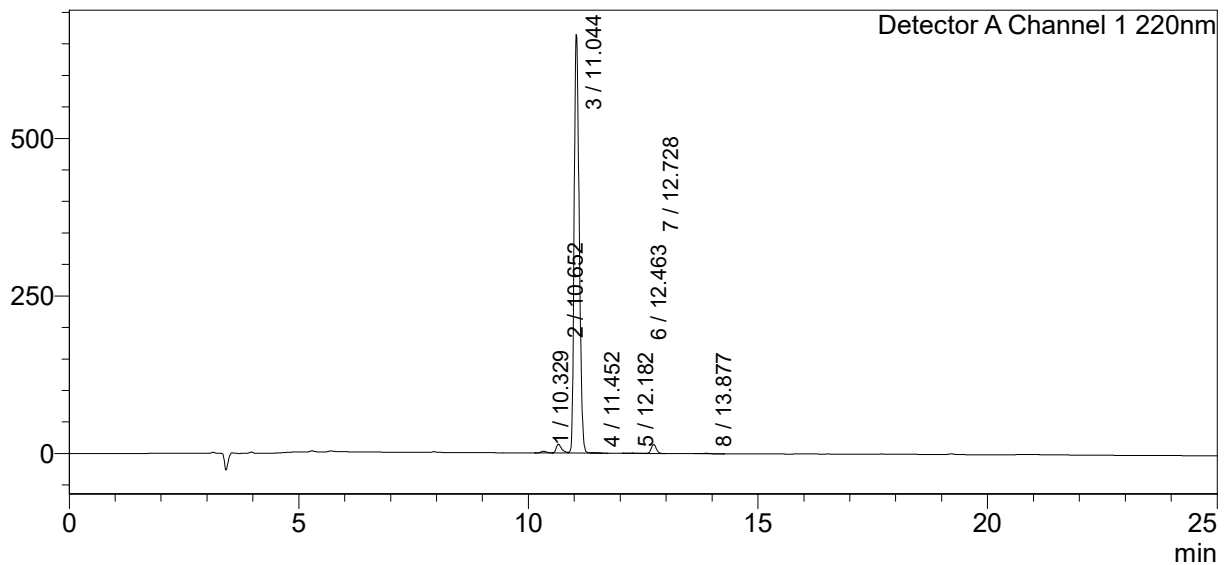

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.329	24443	2816	0.453
2	10.652	119069	14184	2.205
3	11.044	5131204	664311	95.014
4	11.452	2136	320	0.040
5	12.182	1668	196	0.031
6	12.463	5045	327	0.093
7	12.728	110419	14346	2.045
8	13.877	6499	747	0.120
Total		5400482	697249	100.000