

Sample Name : CLIP (86-100)
 Cat. No. :RP20279 Lot. No. :PE1751807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

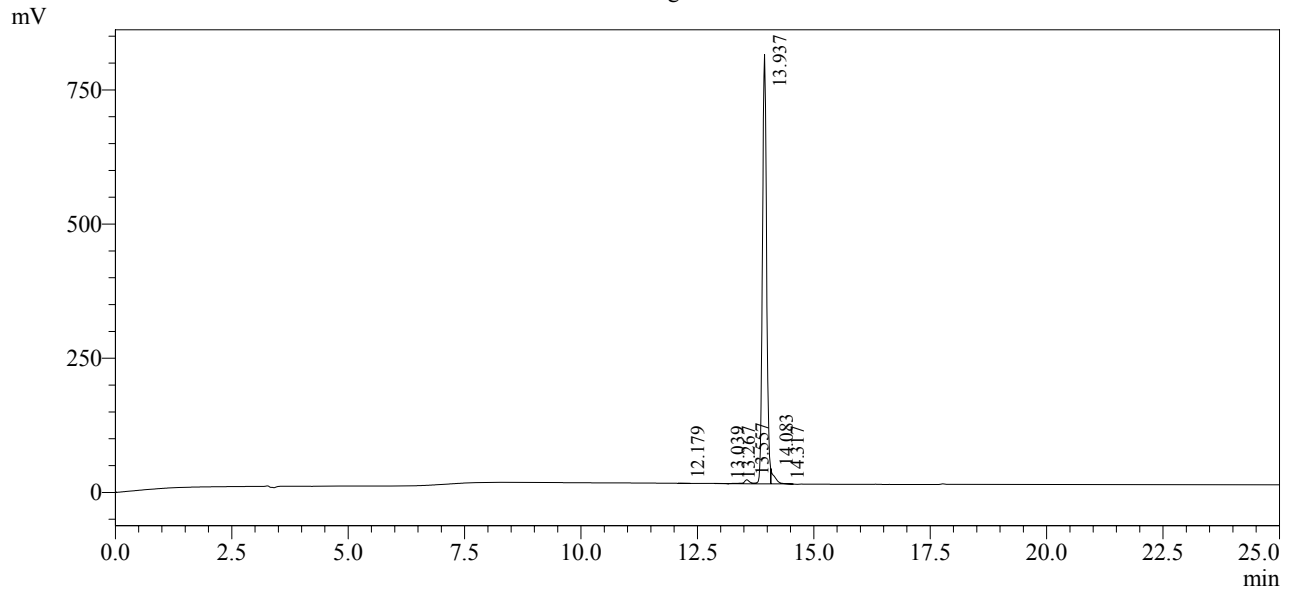

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.179	1817	336	0.035
2	13.039	2814	458	0.054
3	13.267	2474	456	0.048
4	13.557	62607	7401	1.204
5	13.937	4986733	799622	95.924
6	14.083	136608	24888	2.628
7	14.317	5570	1169	0.107
Total		5198622	834331	100.000