

Sample Name : β -Amyloid (1-42), human
 Cat. No. : RP10017
 Lot. No. : PE3801812
 Time Processed : 8:28:51
 Month-Day-Year Processed : 02/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
31.00	Pumps	Pump A B.Conc	5	
31.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

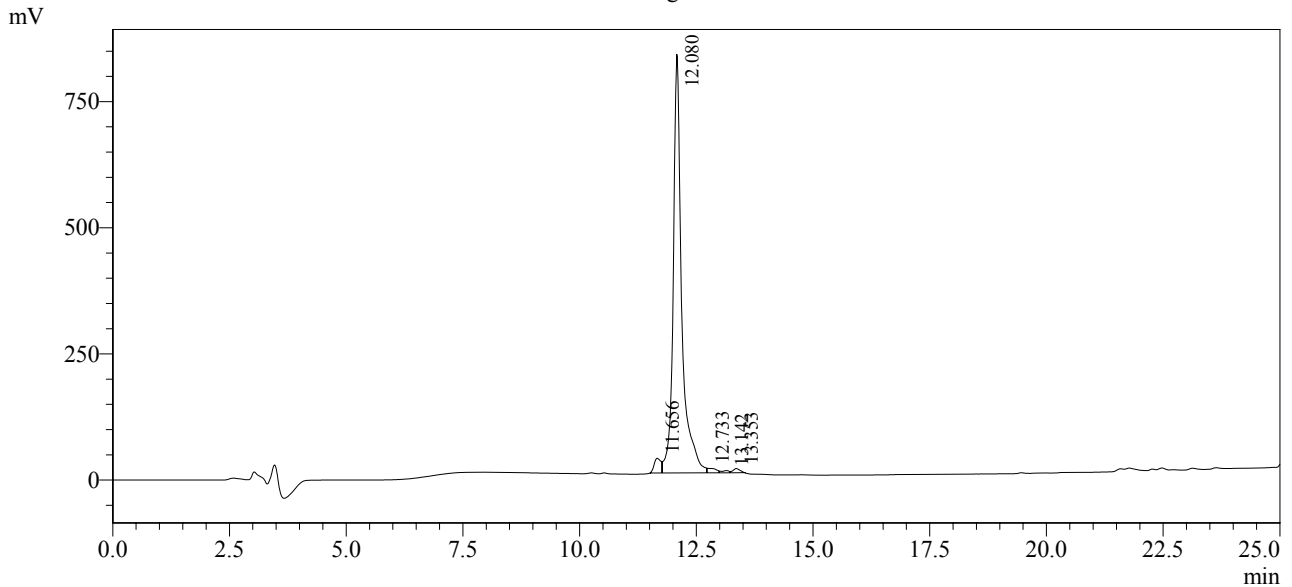

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.656	294808	29123	2.682
2	12.080	10450130	829651	95.064
3	12.733	115905	9050	1.054
4	13.142	46157	4419	0.420
5	13.353	85713	8305	0.780
Total		10992714	880548	100.000