

Sample Name :Protease-Activated Receptor-2, amide
 Cat No. :RP20334
 Lot No. :E7212820L
 Time Processed :3:22:14 PM
 Month-Day-Year Processed :12/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

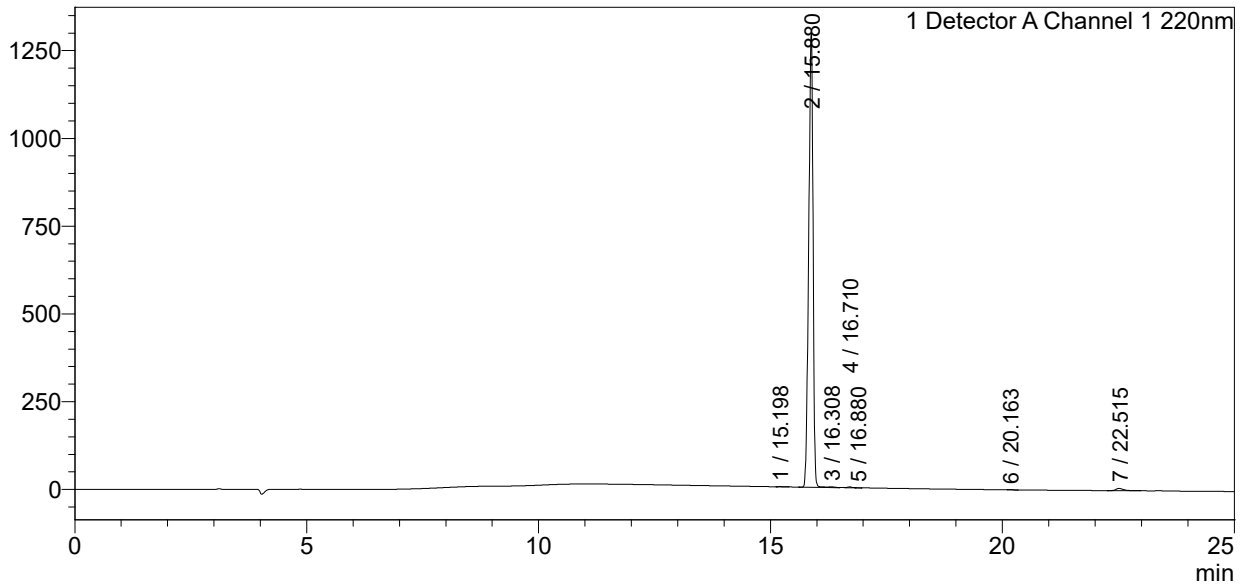

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.198	3368	581	0.040
2	15.880	8371579	1293651	98.580
3	16.308	22268	2054	0.262
4	16.710	19011	2562	0.224
5	16.880	5340	755	0.063
6	20.163	1146	193	0.013
7	22.515	69447	6463	0.818
Total		8492160	1306260	100.000