

Sample Name : Bradykinin (1-7)  
 Cat. No. : RP11133  
 Lot. No. : E7238320B  
 Time Processed : 10:10:35  
 Month-Day-Year Processed : 02/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

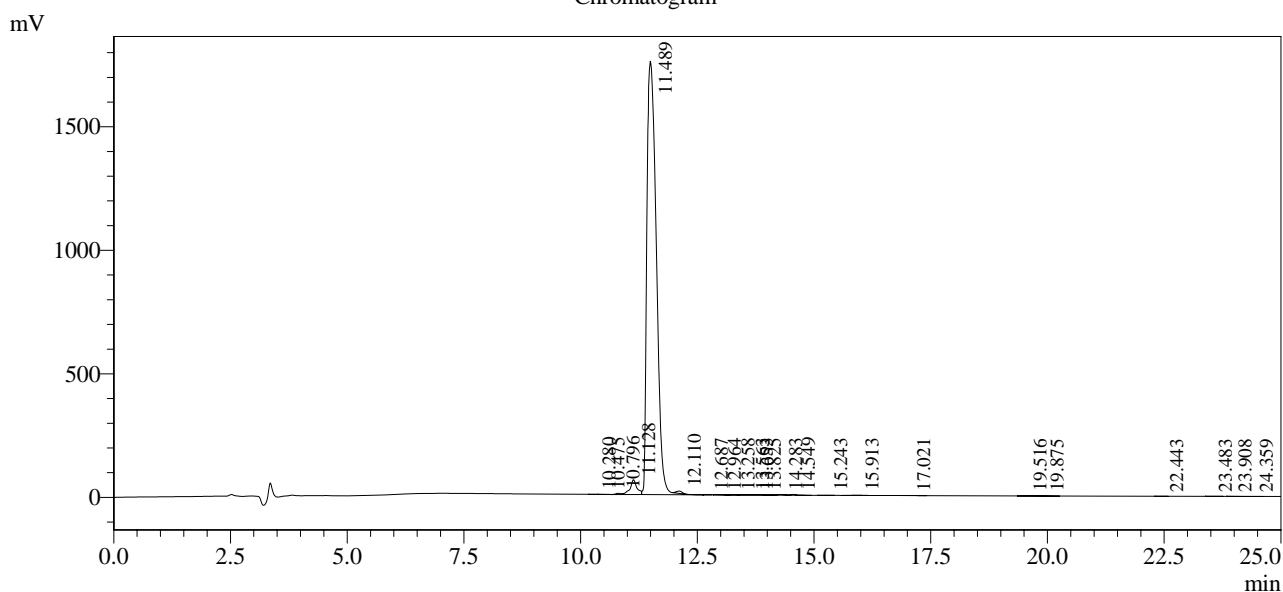

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.280	2190	462	0.009
2	10.475	11233	1578	0.044
3	10.796	40122	4812	0.158
4	11.128	605449	60053	2.381
5	11.489	24561999	1754204	96.598
6	12.110	81035	9450	0.319
7	12.687	1286	250	0.005
8	12.964	6493	918	0.026
9	13.258	2661	409	0.010
10	13.563	4133	384	0.016
11	13.653	2829	425	0.011
12	13.825	6313	522	0.025
13	14.283	25542	2285	0.100
14	14.549	24772	3083	0.097
15	15.243	4728	511	0.019
16	15.913	27100	1299	0.107
17	17.021	7235	336	0.028
18	19.516	4559	344	0.018
19	19.875	1084	36	0.004
20	22.443	1127	167	0.004
21	23.483	1507	126	0.006
22	23.908	1337	118	0.005
23	24.359	2272	223	0.009
Total		25427007	1841995	100.000