

Sample Name :Glucagon (1-29), Human
 Cat No. :RP10772
 Lot No. :E6507521G
 Time Processed :2:35:28
 Month-Day-Year Processed :07/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

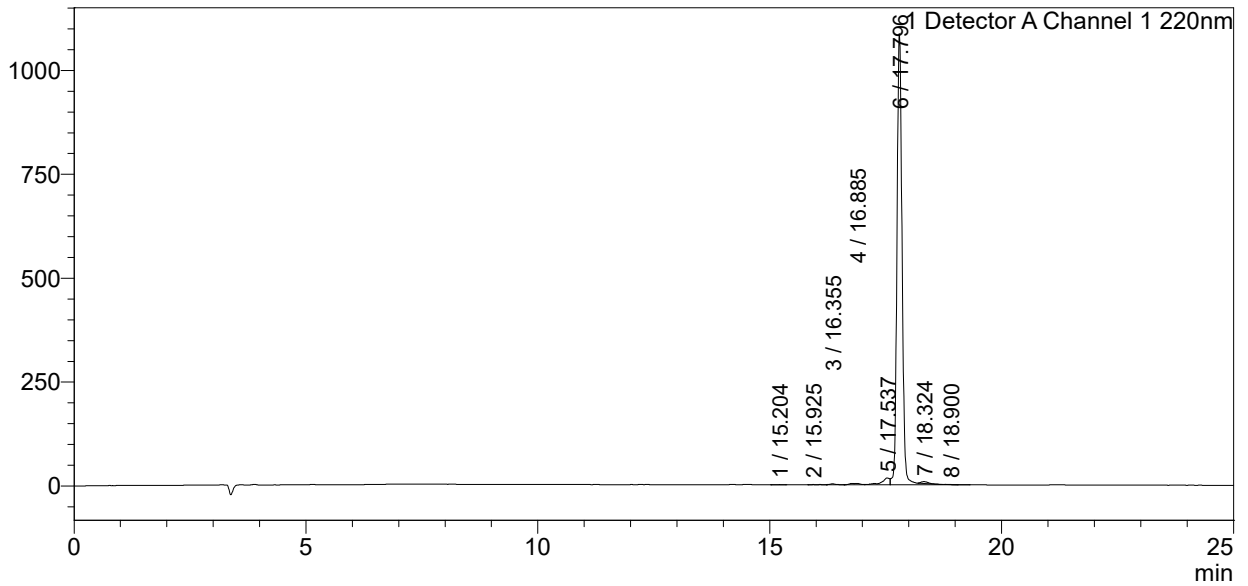

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.204	3912	401	0.045
2	15.925	6384	313	0.074
3	16.355	18819	2072	0.218
4	16.885	48952	3427	0.566
5	17.537	201296	16271	2.328
6	17.796	8312493	1075337	96.150
7	18.324	51866	4547	0.600
8	18.900	1652	268	0.019
Total		8645374	1102636	100.000