

Sample Name: Angiotensin II, human
 Cat. No. : RP11257
 Lot. No. : E0365619H
 Time Processed :0:52:07
 Month-Day-Year Processed :08/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

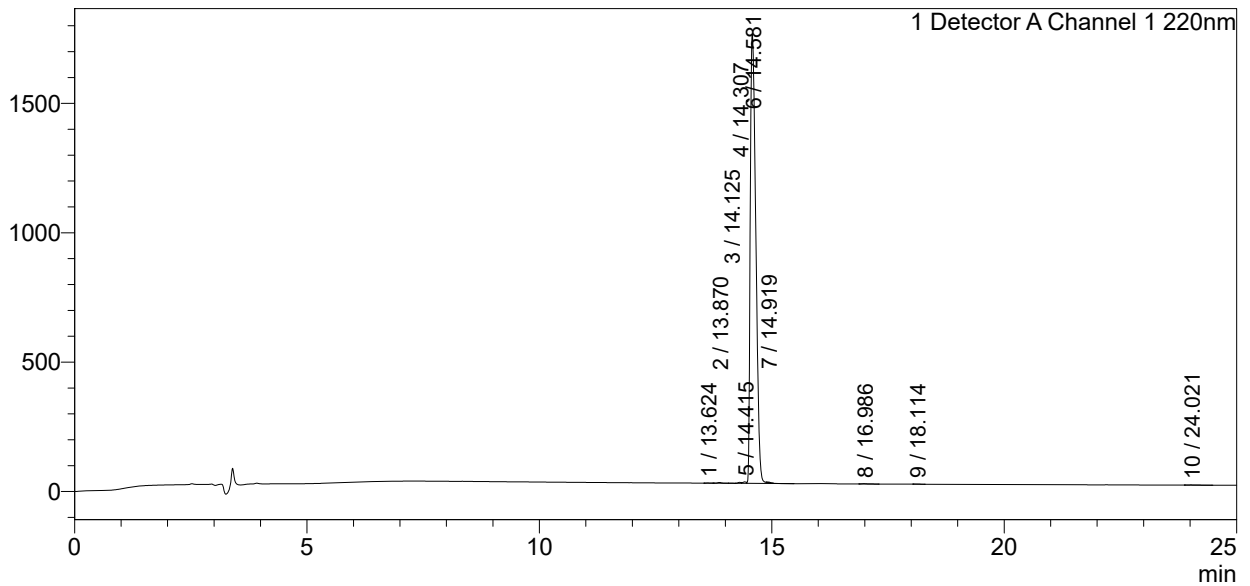

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.624	2886	592	0.020
2	13.870	17607	2937	0.121
3	14.125	1785	364	0.012
4	14.307	17157	3596	0.118
5	14.415	27885	5513	0.192
6	14.581	14424332	1735837	99.365
7	14.919	7934	2037	0.055
8	16.986	8981	1154	0.062
9	18.114	1997	327	0.014
10	24.021	6017	631	0.041
Total		14516582	1752988	100.000