

Sample Name :GHRF (1-44), human
 Cat. No. : RP10734□□
 Lot. No. : PE8991811
 Time Processed :10:55:24
 Month-Day-Year Processed :11/20/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

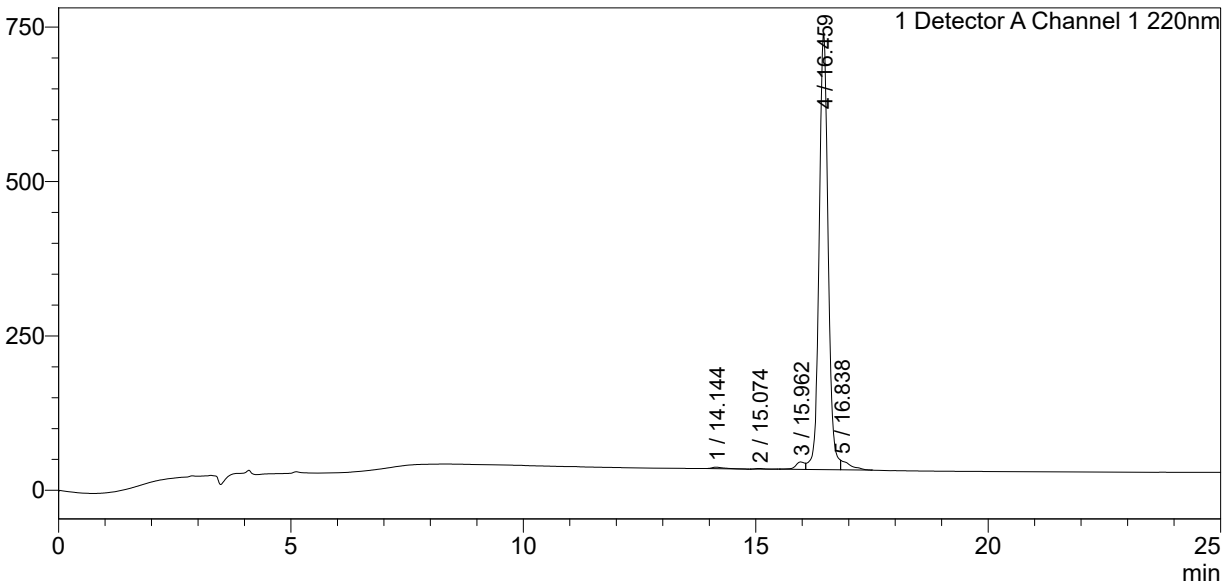

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.144	45313	2390	0.456
2	15.074	13932	1079	0.140
3	15.962	164227	12095	1.651
4	16.459	9508720	706129	95.589
5	16.838	215309	15098	2.164
Total		9947501	736791	100.000