

Sample Name :Eledoisin Related Peptide
Cat. No. : RP10457
Lot. No. : E7087919J
Time Processed :11:06:17
Month-Day-Year Processed : 10/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

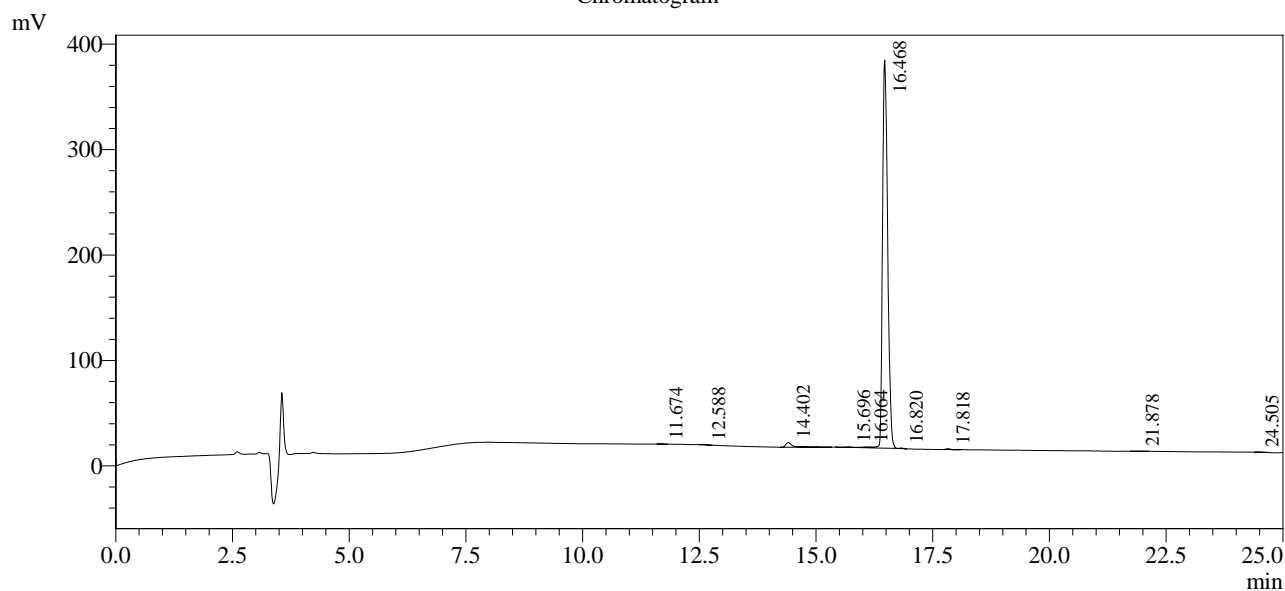

1 Det.A Ch1 / 220nm
Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.674	1811	233	0.063
2	12.588	2636	406	0.091
3	14.402	49617	4574	1.718
4	15.696	7169	527	0.248
5	16.064	11773	911	0.408
6	16.468	2801267	368271	96.996
7	16.820	2951	622	0.102
8	17.818	5927	897	0.205
9	21.878	2087	216	0.072
10	24.505	2787	369	0.097
Total		2888026	377025	100.000