

Sample Name :HPV16 E7(86-93)  
 Cat No. :RP20499  
 Lot No. :E4974619I  
 Time Processed :10:21:45  
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

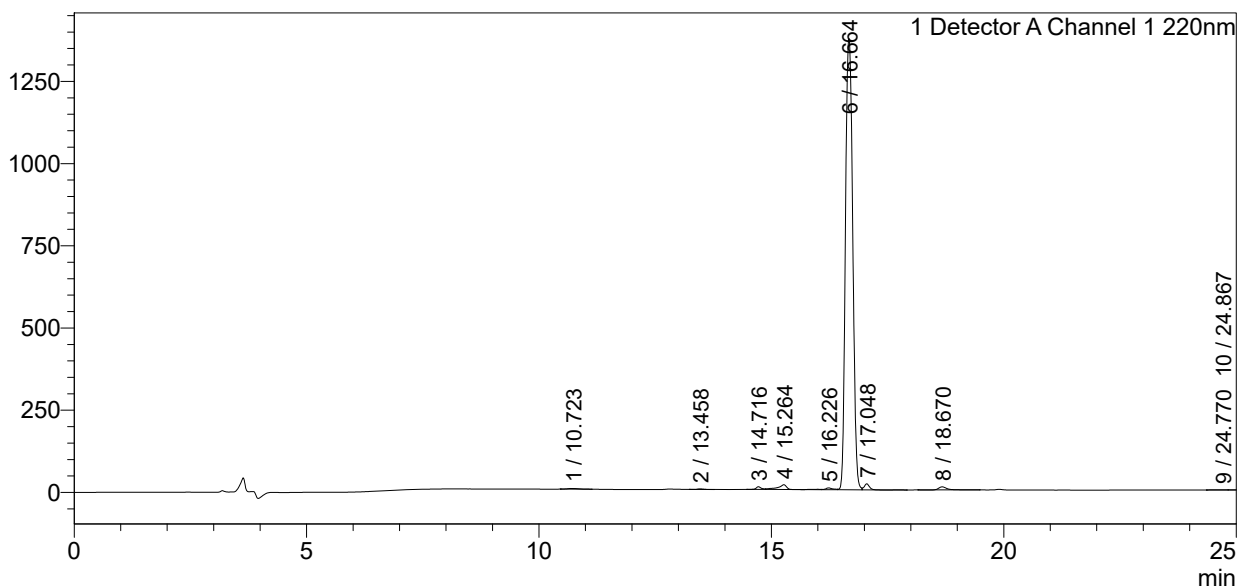

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.723	34551	2336	0.224
2	13.458	14730	1673	0.095
3	14.716	63531	8160	0.411
4	15.264	205806	14558	1.331
5	16.226	56504	5521	0.366
6	16.664	14824372	1372176	95.905
7	17.048	139792	18333	0.904
8	18.670	110330	9323	0.714
9	24.770	5556	337	0.036
10	24.867	2256	306	0.015
Total		15457427	1432723	100.000