

Sample Name : Neurotensin (8-13)

Cat. No. : RP10442 Lot. No. : PE9021712

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

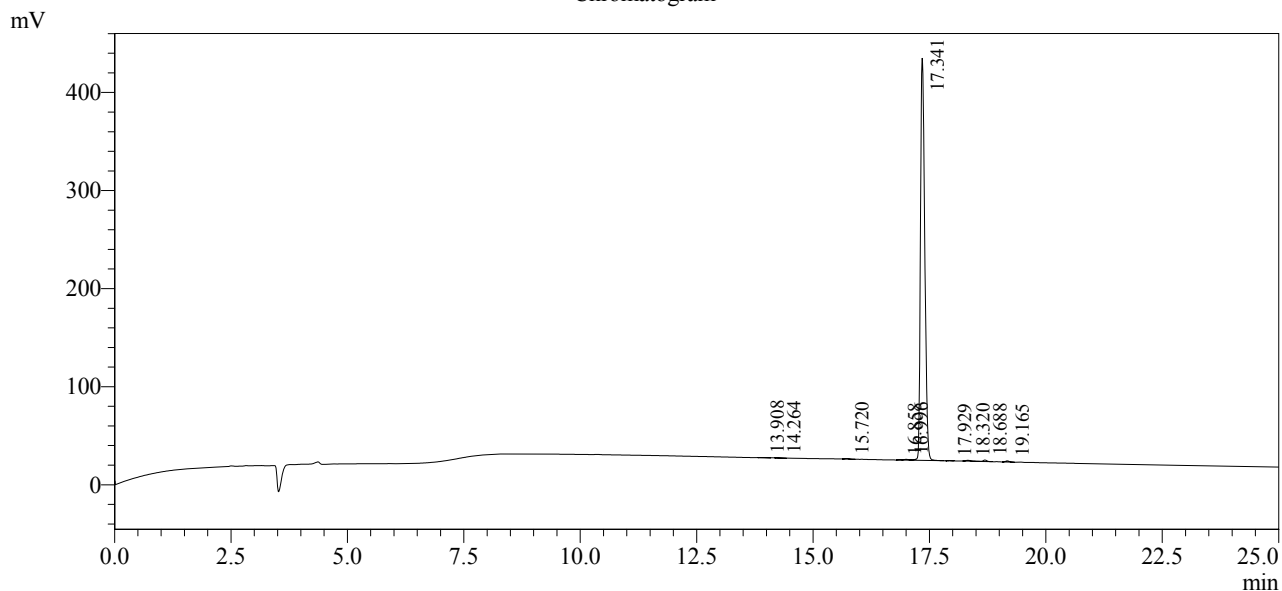

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.908	2129	355	0.080
2	14.264	2508	484	0.094
3	15.720	2810	543	0.105
4	16.858	1765	330	0.066
5	16.996	6121	848	0.229
6	17.341	2638441	409909	98.613
7	17.929	1167	236	0.044
8	18.320	6097	914	0.228
9	18.688	8200	1527	0.306
10	19.165	6322	1177	0.236
Total		2675561	416324	100.000