

Sample Name: Mastoparan
 Cat No. : RP10465
 Lot No. : E6992519J
 Time Processed: 8:50:19 AM
 Month-Day-Year Processed : 10/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

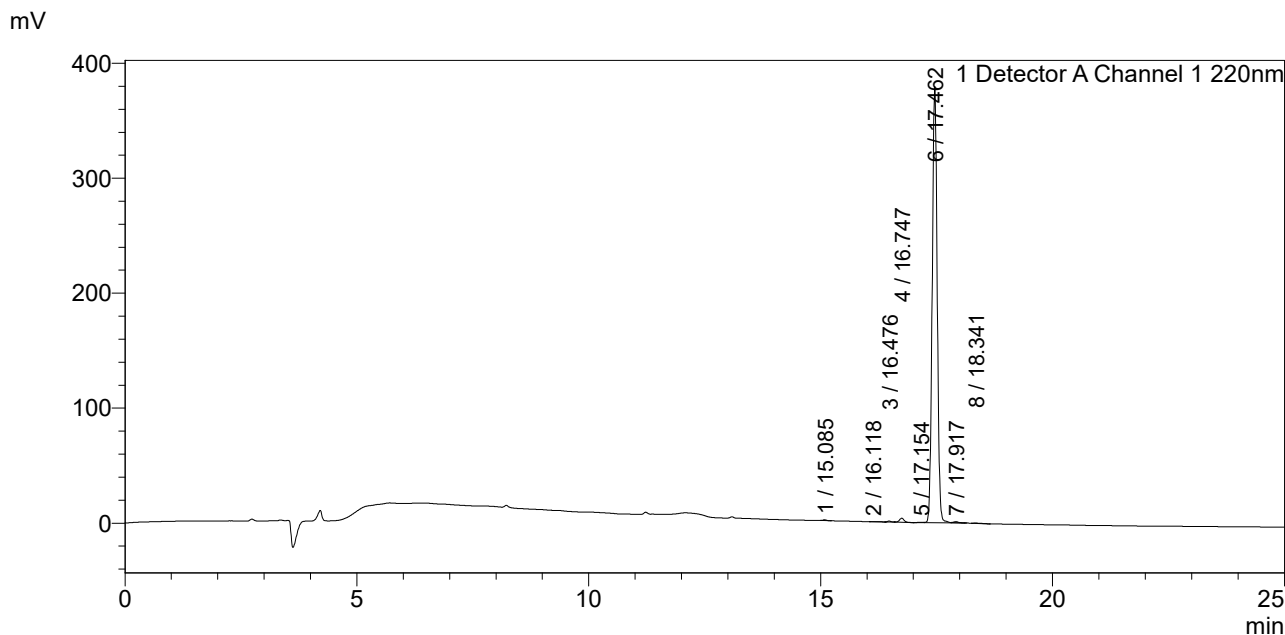

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.085	3617	711	0.126
2	16.118	1399	77	0.049
3	16.476	4132	848	0.144
4	16.747	24667	3561	0.858
5	17.154	2891	405	0.101
6	17.462	2827658	379791	98.380
7	17.917	6516	992	0.227
8	18.341	3330	359	0.116
Total		2874211	386744	100.000