

Sample Name :Proctolin  
 Cat. No. : RP10475  
 Lot. No. : E7501720A  
 Time Processed :7:01:12  
 Month-Day-Year Processed : 01/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

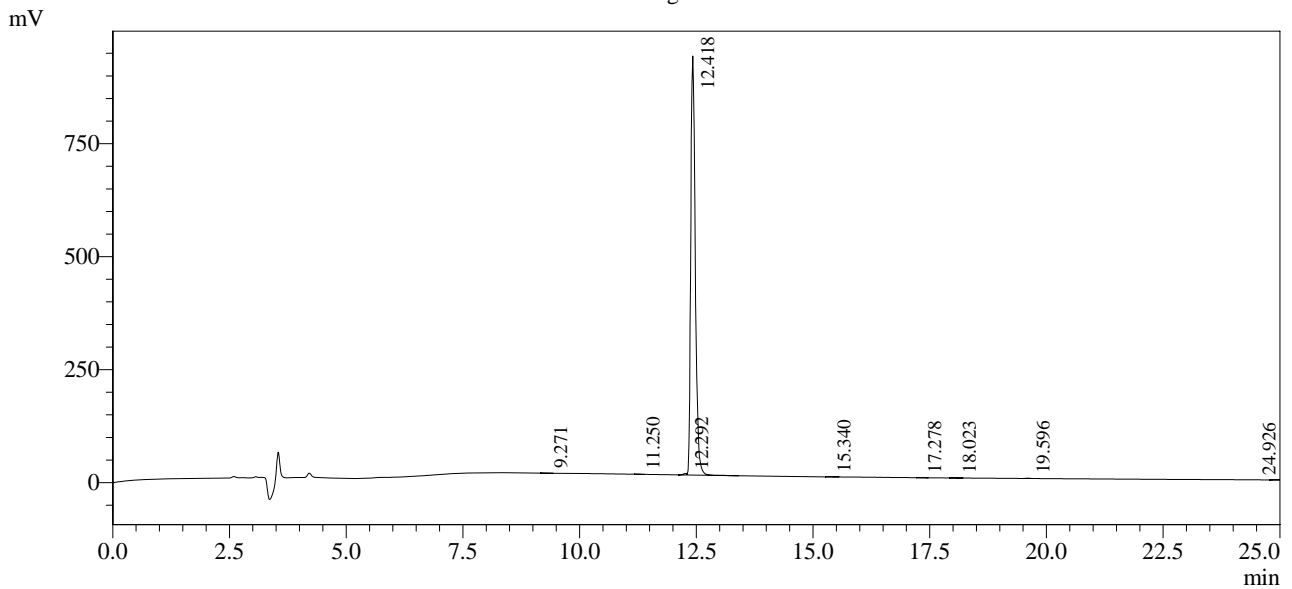

1 Det. A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.271	1797	230	0.028
2	11.250	1524	289	0.024
3	12.292	18137	3223	0.287
4	12.418	6289128	927500	99.460
5	15.340	2863	379	0.045
6	17.278	1166	107	0.018
7	18.023	1727	192	0.027
8	19.596	4923	664	0.078
9	24.926	1983	287	0.031
Total		6323250	932870	100.000