

Sample Name: Crustacean Cardioactive Peptide (CCAP)

Cat. No. : RP10572

Lot. No. : E5714219F

Time Processed : 9:00:54

Month-Day-Year Processed : 07/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

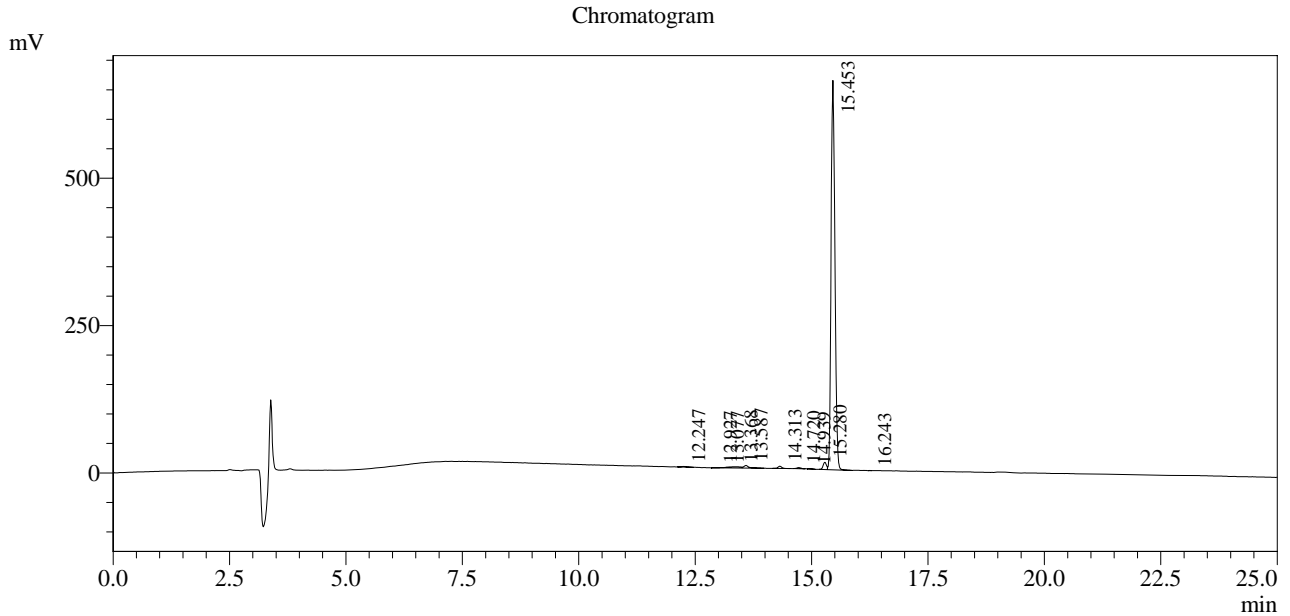

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.247	6360	975	0.159
2	12.927	1726	290	0.043
3	13.077	3631	616	0.091
4	13.368	41237	2095	1.032
5	13.587	36139	4531	0.904
6	14.313	21566	3823	0.540
7	14.720	11774	1848	0.295
8	14.939	2480	458	0.062
9	15.280	61202	12326	1.532
10	15.453	3808996	660406	95.332
11	16.243	409	197	0.010
Total		3995519	687566	100.000