

Sample Name : [Leu5]-Enkephalin
 Cat No. : RP10884
 Lot No. : E4938320L
 Time Processed : 19:25:25
 Month-Day-Year Processed : 12/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

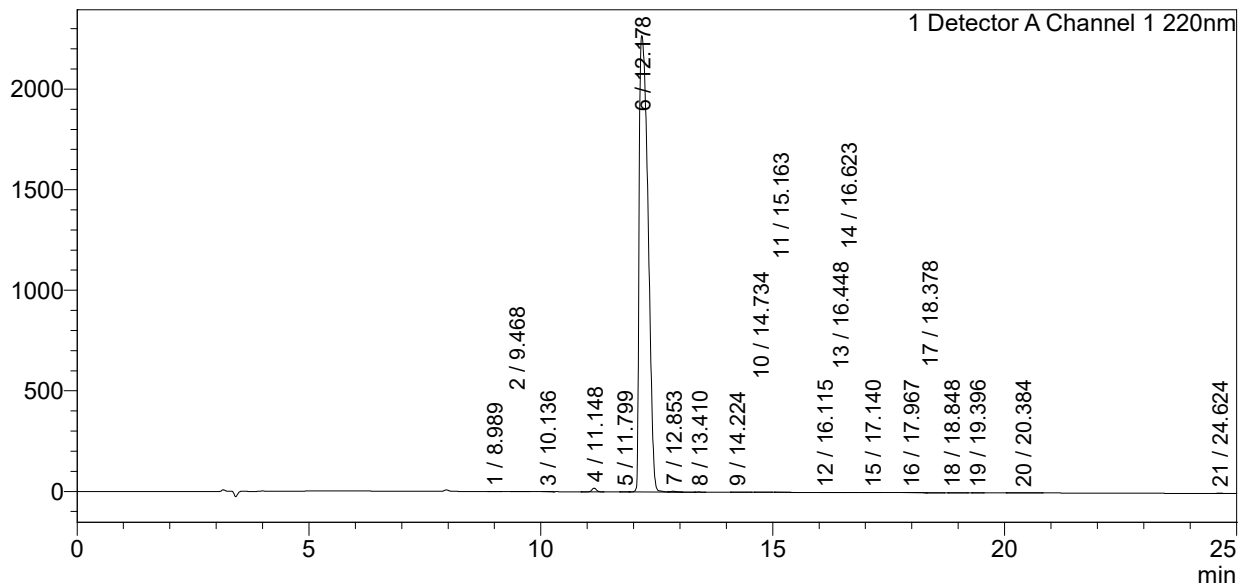

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.989	1394	207	0.005
2	9.468	5768	775	0.019
3	10.136	2445	391	0.008
4	11.148	121198	18034	0.400
5	11.799	2210	301	0.007
6	12.178	30092535	2268838	99.249
7	12.853	25143	3308	0.083
8	13.410	2587	464	0.009
9	14.224	2199	176	0.007
10	14.734	1511	103	0.005
11	15.163	4535	466	0.015
12	16.115	1121	94	0.004
13	16.448	3433	469	0.011
14	16.623	5881	660	0.019

Peak#	Ret. Time	Area	Height	Area%
15	17.140	2440	227	0.008
16	17.967	6122	480	0.020
17	18.378	1702	68	0.006
18	18.848	1236	74	0.004
19	19.396	1223	161	0.004
20	20.384	24233	1032	0.080
21	24.624	11367	1164	0.037
Total		30320285	2297491	100.000