

Sample Name :Tuftsin
 Cat No. :RP10624
 Lot No. :E6858020H
 Time Processed :7:56:58
 Month-Day-Year Processed :08/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 0 |
| 5.00 | Pumps | Solvent B Conc. | 0 |
| 20.00 | Pumps | Solvent B Conc. | 30 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 31.00 | Pumps | Solvent B Conc. | 95 |
| 31.01 | Pumps | Solvent B Conc. | 0 |
| 40.00 | Pumps | Solvent B Conc. | 0 |
| 40.01 | Controller | Stop | |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

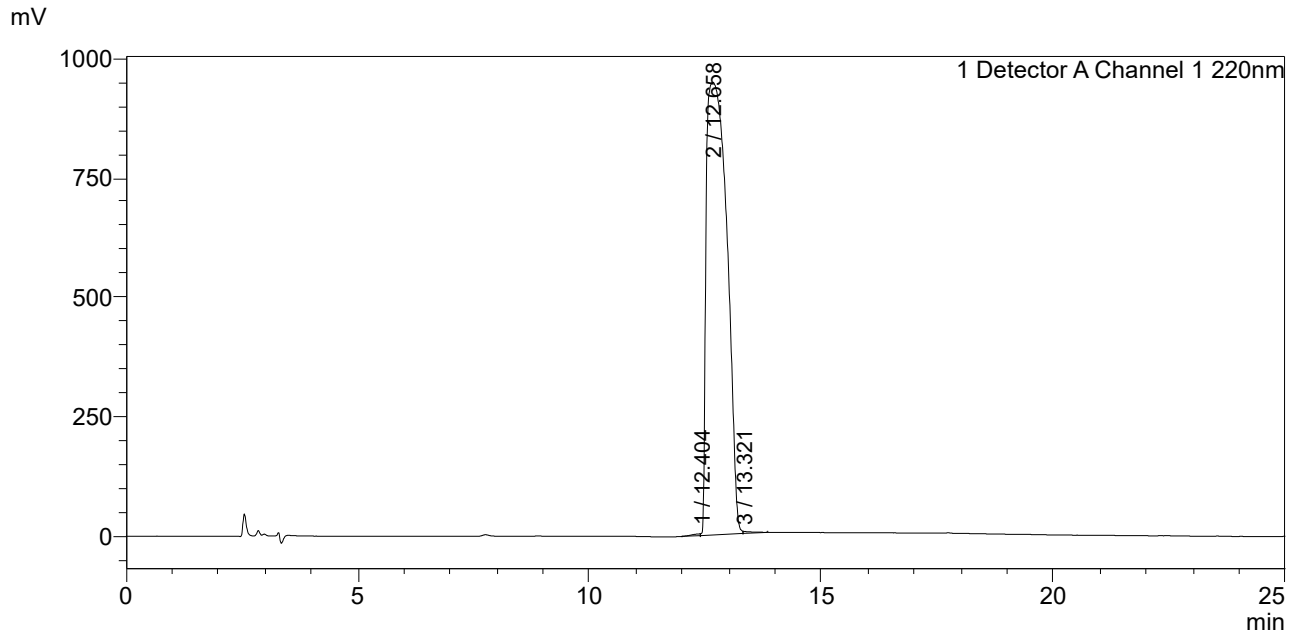

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|--------|---------|
| 1 | 12.404 | 50989 | 3724 | 0.174 |
| 2 | 12.658 | 29139112 | 948162 | 99.626 |
| 3 | 13.321 | 58447 | 4589 | 0.200 |
| Total | | 29248547 | 956476 | 100.000 |