

Sample Name :HIV-1 TAT (48-60)
 Cat No. :RP20423
 Lot No. :E6898719K
 Time Processed :15:37:38
 Month-Day-Year Processed :11/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

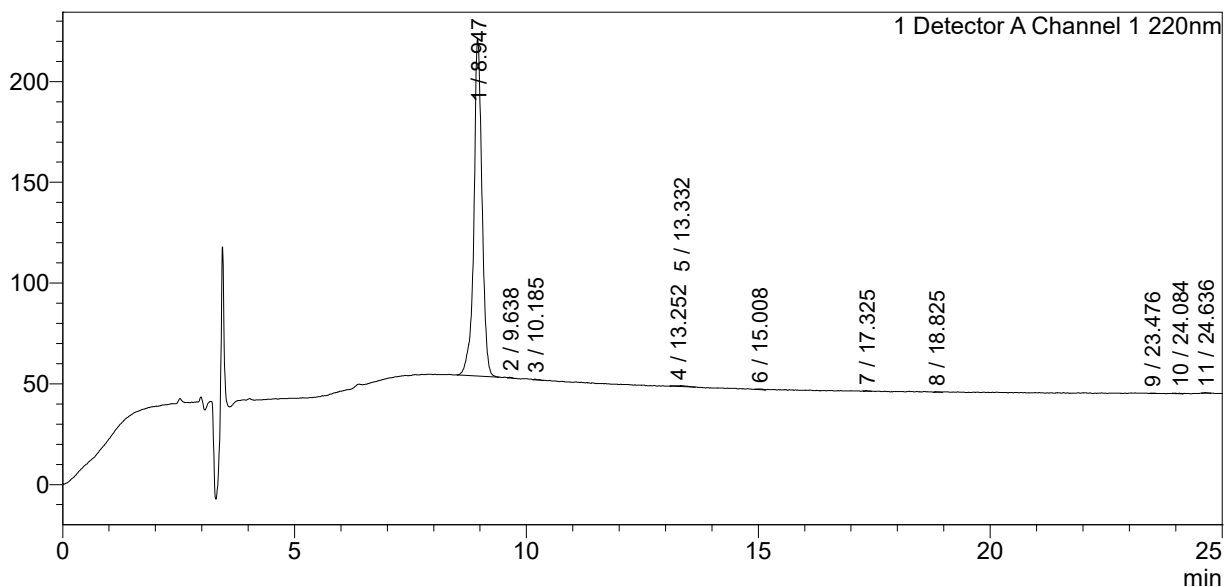

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.947	2047509	167735	98.872
2	9.638	1634	349	0.079
3	10.185	1880	406	0.091
4	13.252	2788	380	0.135
5	13.332	6009	528	0.290
6	15.008	2670	328	0.129
7	17.325	1806	363	0.087
8	18.825	1651	263	0.080
9	23.476	1630	215	0.079
10	24.084	1971	228	0.095
11	24.636	1324	268	0.064
Total		2070873	171063	100.000