


Mass Spectrum

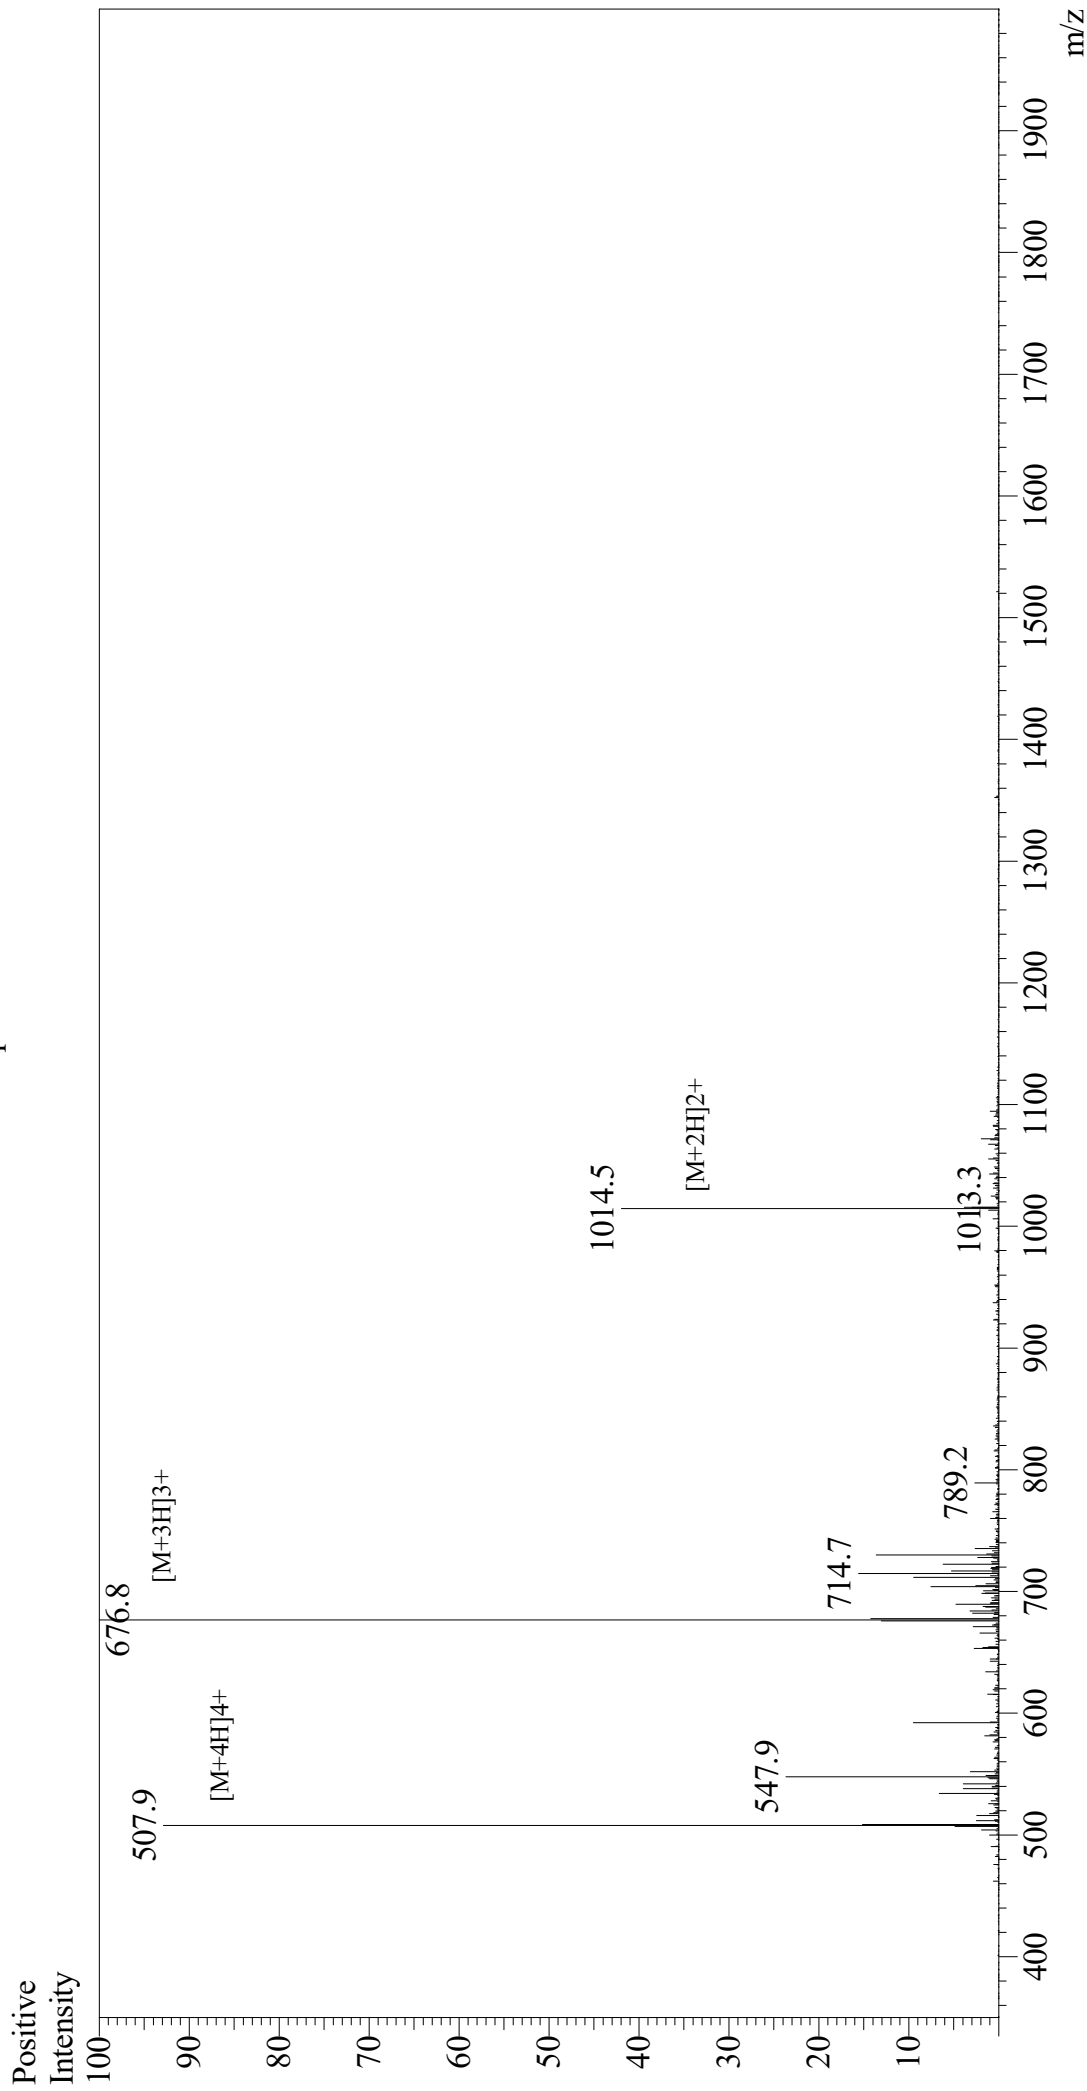

Sample Information
Month-Day Processed : 08/26/21
Time Processed : 8:54:41
Injection Volume : 0.2
Sample Name : Apamin
Cat No : RP11002
Lot No : E2111021G
Theoretical MW : 2027.30
Observed MW : 2027.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH