

Sample Name :Arg-Gly-Asp-Ser
 Cat No. :RP10861
 Lot No. :E2111620D
 Time Processed :11:48:28
 Month-Day-Year Processed :04/07/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

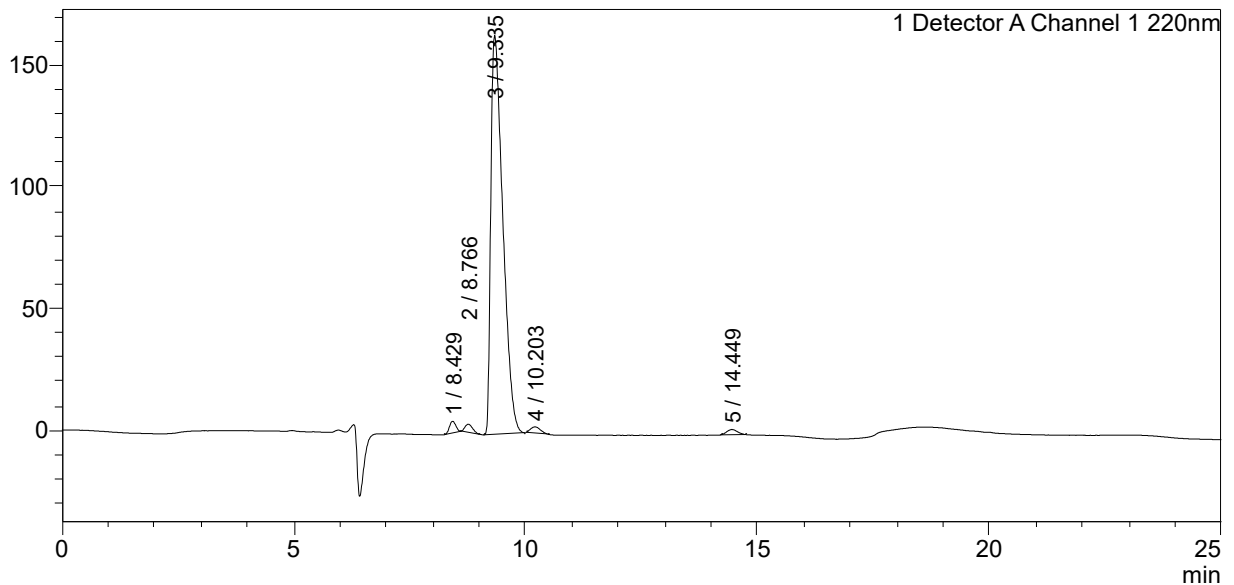

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.429	46046	4823	1.486
2	8.766	37366	3338	1.205
3	9.335	2945530	164080	95.027
4	10.203	36213	2499	1.168
5	14.449	34515	2147	1.114
Total		3099669	176888	100.000