


Mass Spectrum

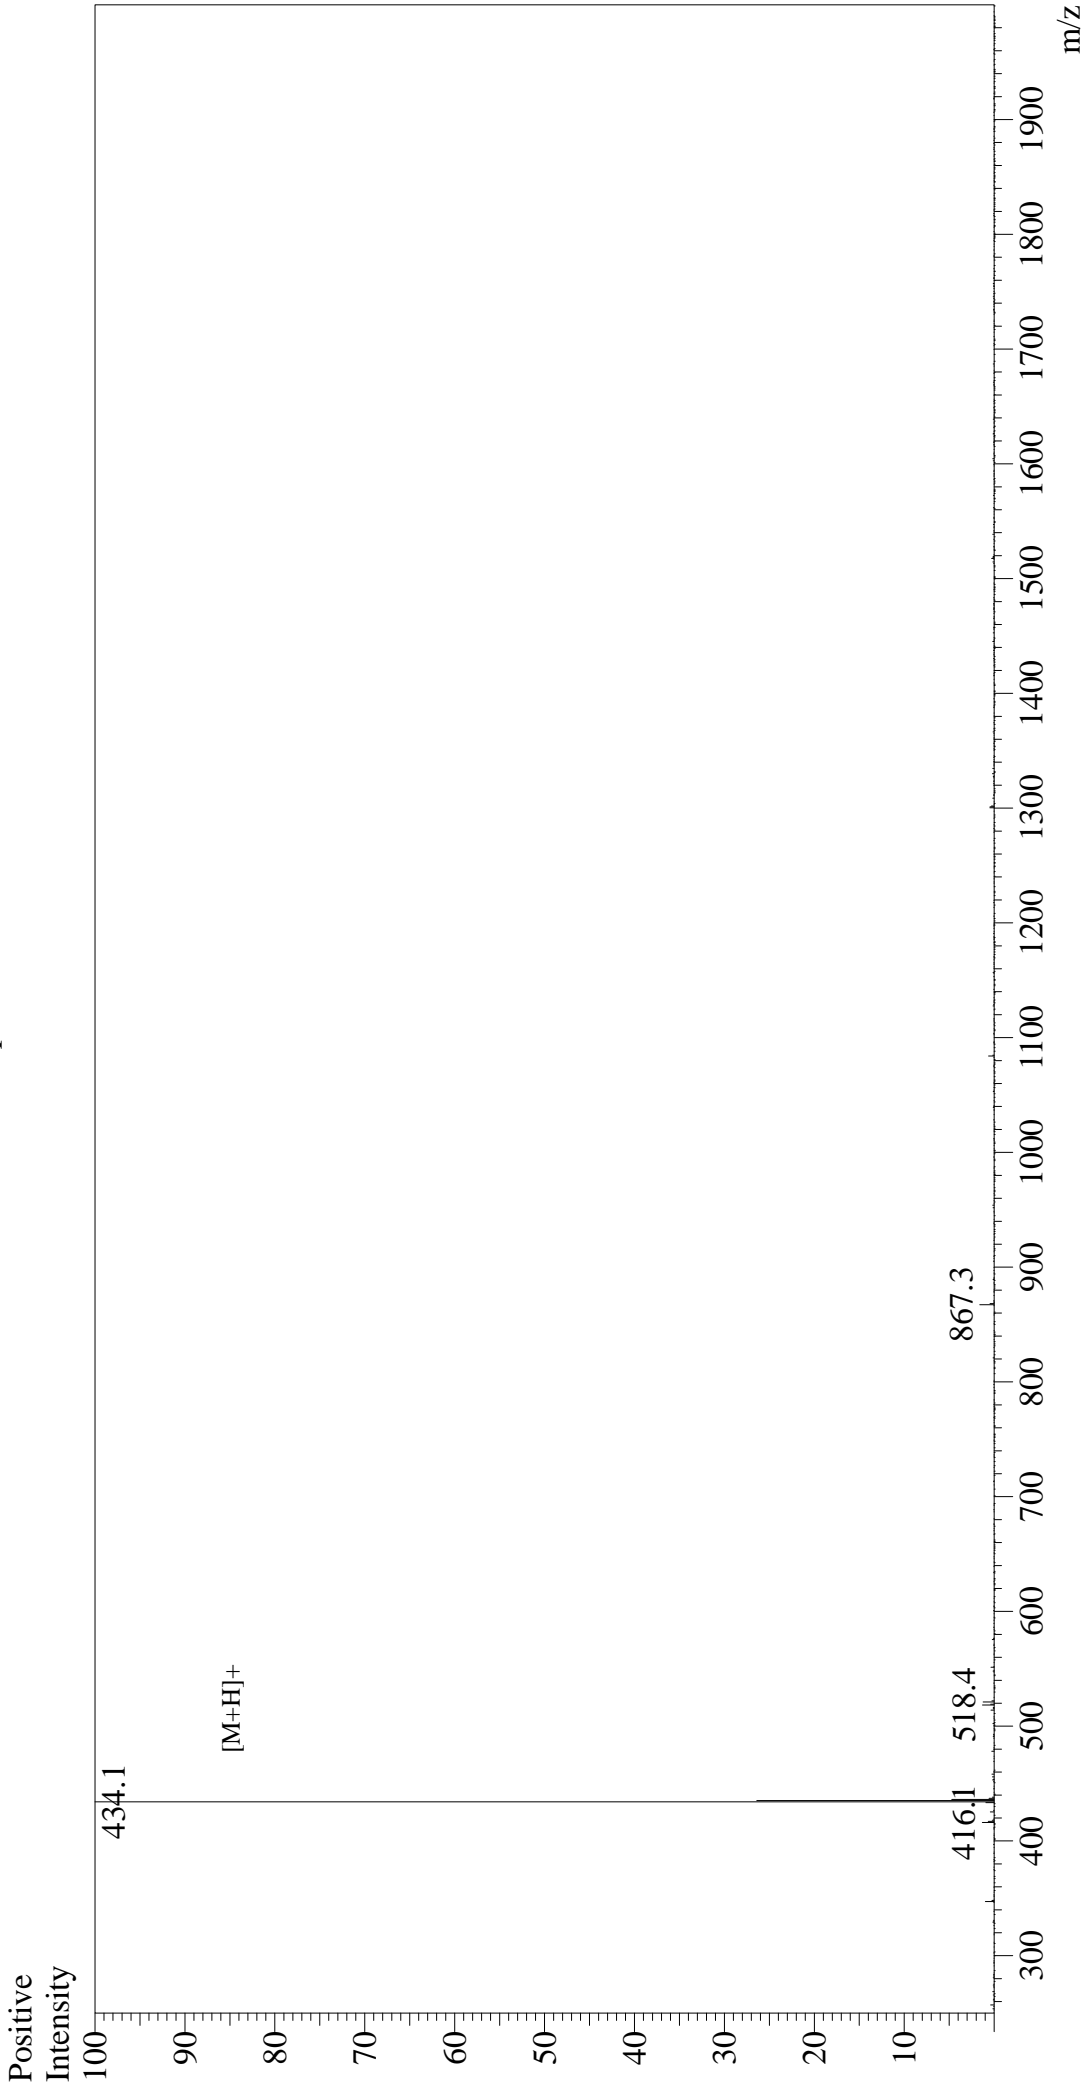

Sample Information

Acquired by : Gary
Month-Day Processed : 04/07/20
Time Processed : 8:32:11
Injection Volume : 0.3
Sample Name : Arg-Gly-Asp-Ser
Cat. No. : RP10861
Lot. No. : E2111620D
Theoretical MW : 433.42
Observed MW : 433.1

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH