


Mass Spectrum

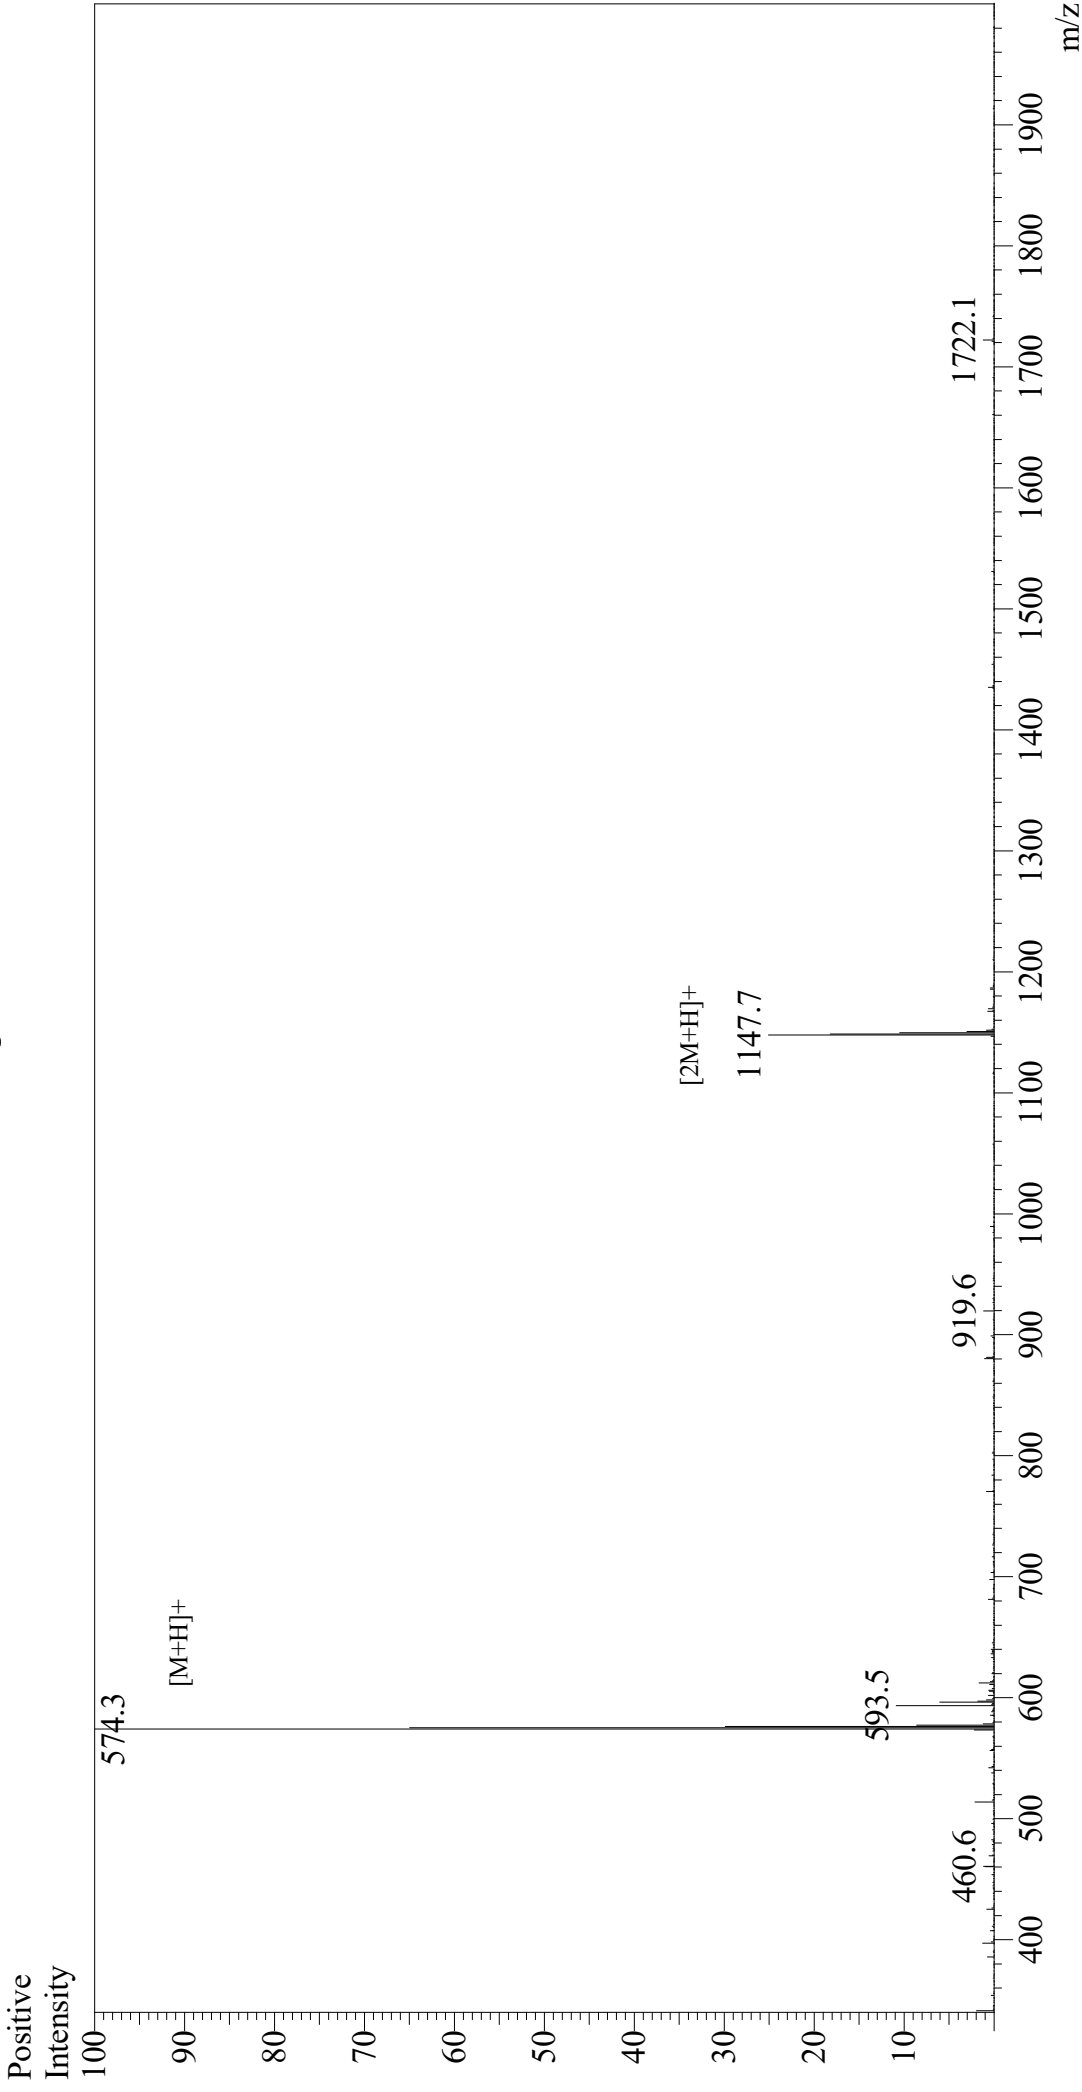

Sample Information

Month-Day Processed : 06/17/21
Time Processed : 9:38:57
Injection Volume : 0.2
Sample Name : [Met5]-Enkephalin
Cat No. : RP10886
Lot No. : E8884821F
Theoretical MW : 573.66
Observed MW : 573.3

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH