


Mass Spectrum

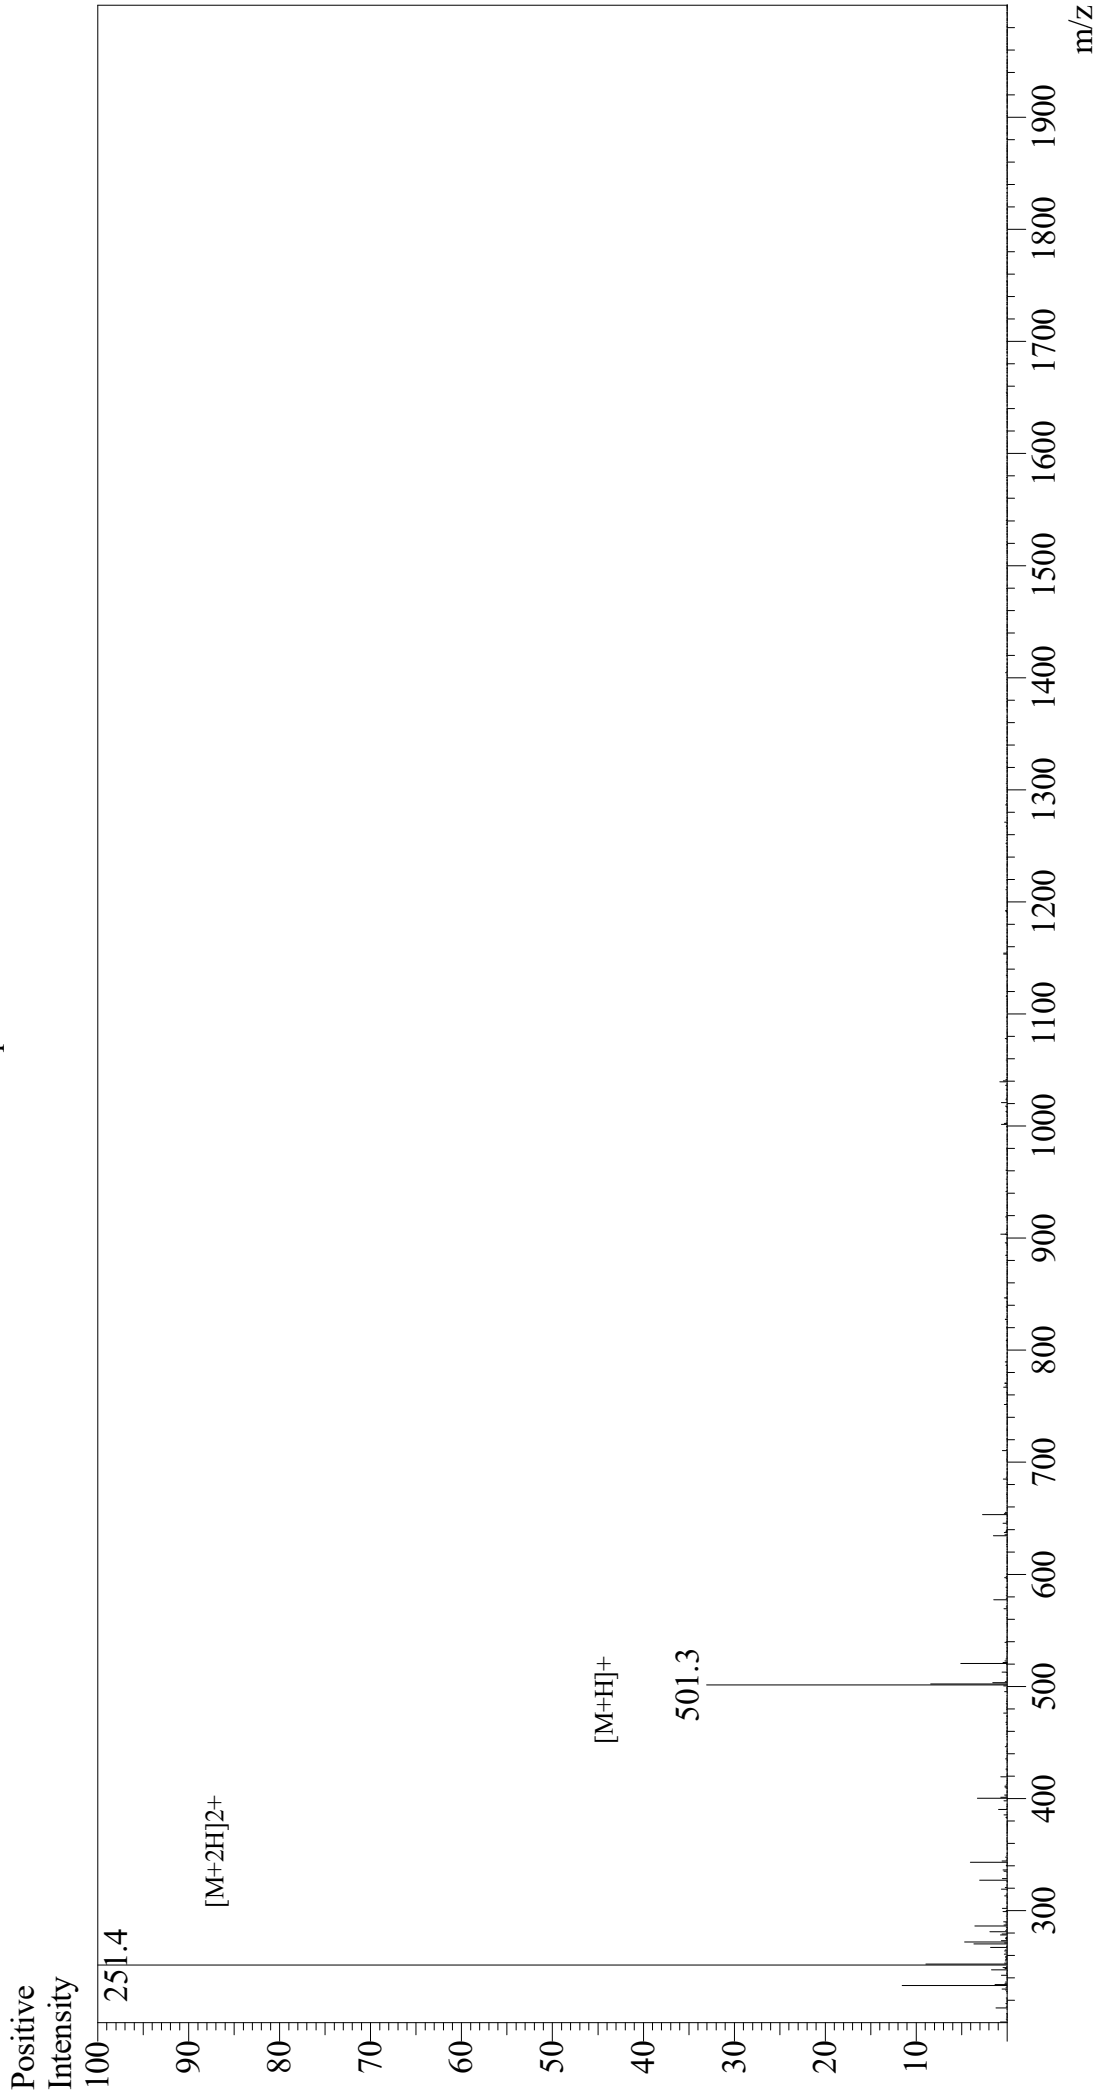

Sample Information
Month-Day Processed : 02/06/21
Time Processed : 9:41:13 PM
Injection Volume : 0.5
Sample Name : Tuftsin
Cat No. : RP10624
Lot No. : E7753321B
Theoretical MW : 500.60
Observed MW : 500.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH