

Sample Name : Arg-Gly-Asp-Cys
 Cat No.: RP10860
 Lot No.: E1564819I
 Time Processed : 8:05:11
 Month-Day-Year Processed : 09/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

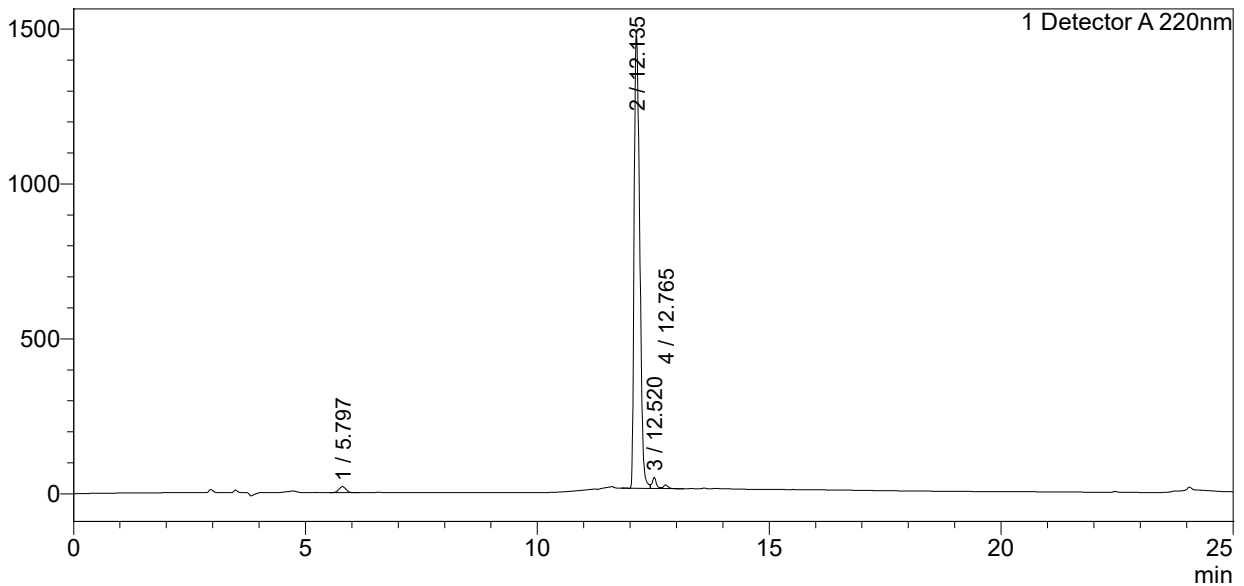

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.797	205110	19526	1.597
2	12.135	12324845	1464241	95.961
3	12.520	226598	36052	1.764
4	12.765	87078	12344	0.678
Total		12843632	1532163	100.000