

Sample Name : Fibronectin Active Fragment Control
 Cat. No. : RP20347
 Lot. No. : E4962119I
 Time Processed :12:58:50
 Month-Day-Year Processed :09/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	25	
40.00	Pumps	Pump B Conc.	25	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

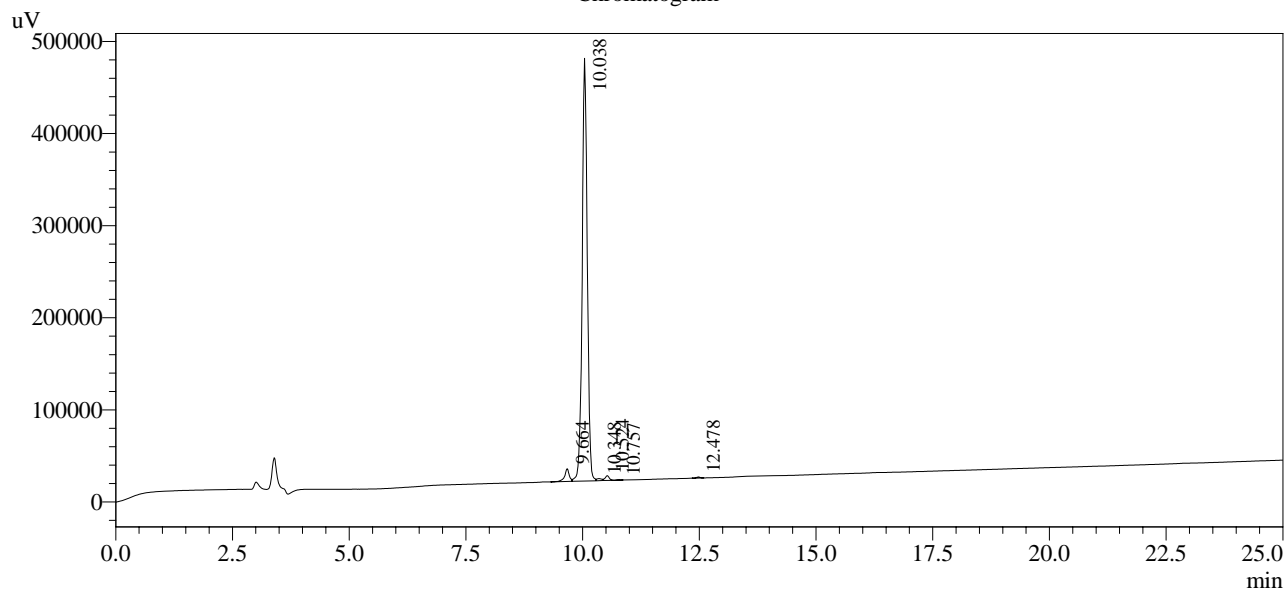

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.664	95873	13861	2.644
2	10.038	3472291	459074	95.775
3	10.348	16011	2237	0.442
4	10.524	32708	5163	0.902
5	10.757	2046	406	0.056
6	12.478	6540	1220	0.180
Total		3625470	481960	100.000