

Sample Name : Bid BH3 Peptide
 Cat. No. : RP20440
 Lot. No. : PE9711706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

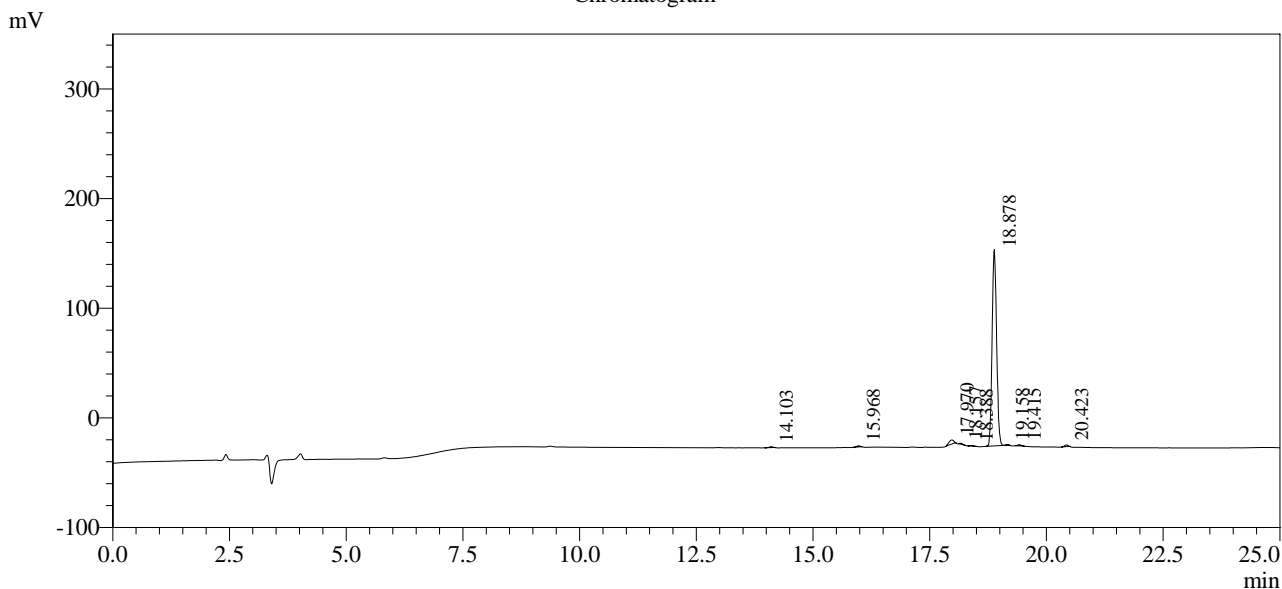

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.103	4731	886	0.377
2	15.968	5564	1018	0.444
3	17.970	27144	3766	2.164
4	18.157	3694	803	0.295
5	18.388	3249	551	0.259
6	18.878	1193773	179046	95.176
7	19.158	2673	695	0.213
8	19.415	5527	998	0.441
9	20.423	7927	1512	0.632
Total		1254283	189274	100.000