

Sample Name :PAR2 AP
 Cat No. :RP19975
 Lot No. :E4898419I
 Time Processed :7:31:13
 Month-Day-Year Processed :09/18/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

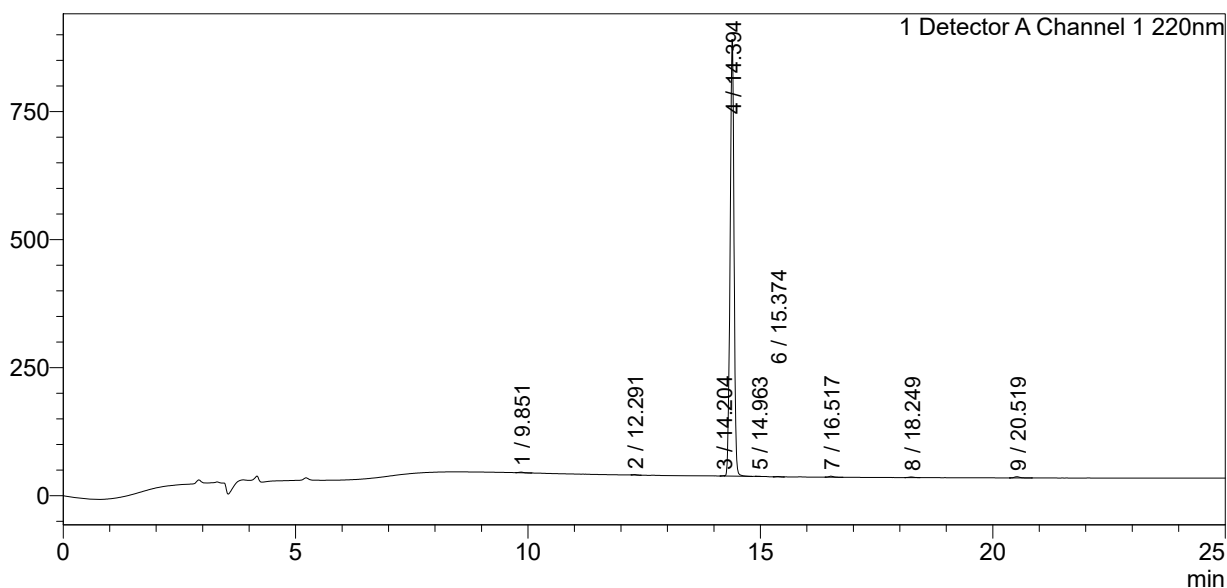

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.851	7882	1254	0.157
2	12.291	4373	881	0.087
3	14.204	1885	526	0.038
4	14.394	4946921	852630	98.783
5	14.963	1109	308	0.022
6	15.374	4165	765	0.083
7	16.517	13449	1932	0.269
8	18.249	8912	1163	0.178
9	20.519	19165	2338	0.383
Total		5007862	861797	100.000