

Sample Name :Thyrotropin-Releasing Hormone (TRH)
 Cat. No. :RP10112
 Lot. No. :E0934519G
 Time Processed : 13:39:36
 Month-Day-Year Processed : 07/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

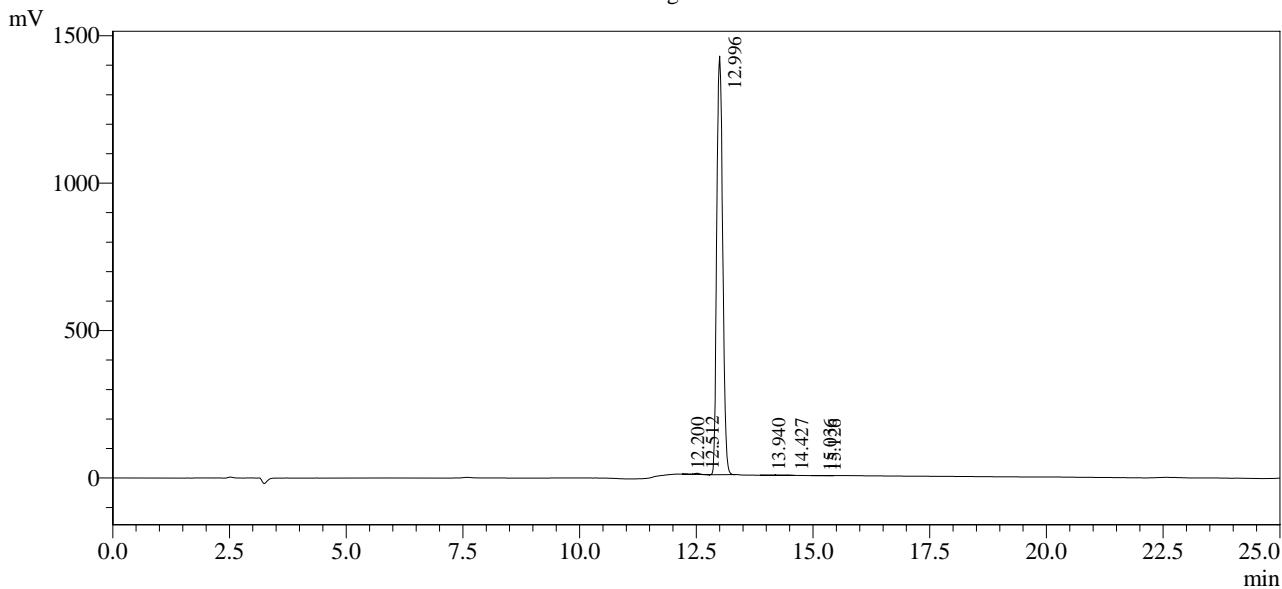

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.200	322	0	0.003
2	12.512	27788	3684	0.219
3	12.996	12631738	1420029	99.677
4	13.940	1017	86	0.008
5	14.427	8165	792	0.064
6	15.036	1234	197	0.010
7	15.126	2396	258	0.019
Total		12672661	1425045	100.000