

Sample Name :N-Formyl-Nle-Leu-Phe-Nle-Tyr-Lys
 Cat. No. : RP12959
 Lot. No. : PE1541808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

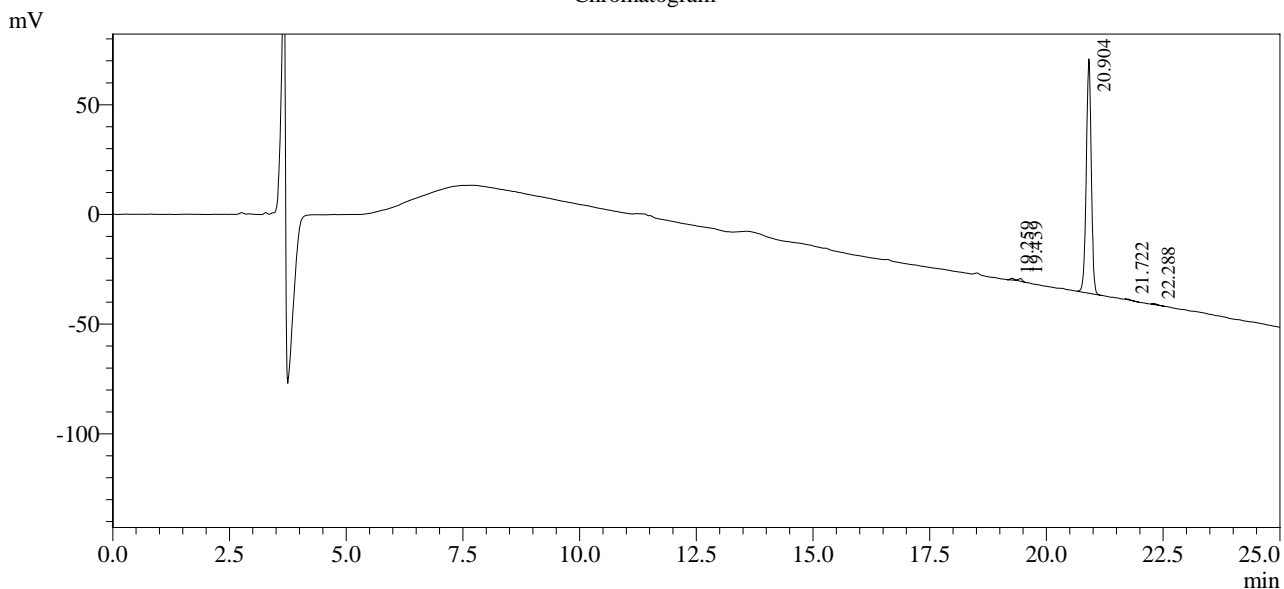

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	19.259	4092	759	0.505
2	19.439	6383	1228	0.787
3	20.904	795596	106859	98.085
4	21.722	2032	275	0.250
5	22.288	3023	362	0.373
Total		811126	109482	100.000