

Sample Name : PLP(139-151)  
 Cat. No. : RP10550  
 Lot. No. : E5697719F  
 Time Processed : 7:01:53  
 Month-Day-Year Processed : 06/29/2019  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

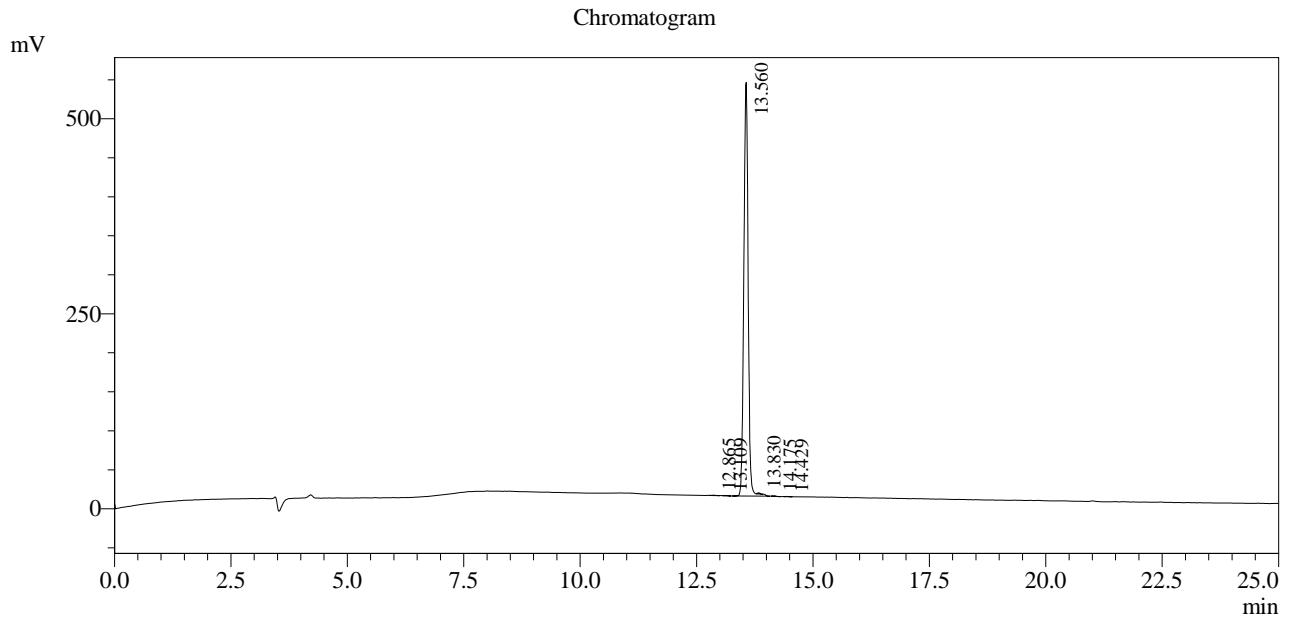

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.865	2676	496	0.078
2	13.109	1443	261	0.042
3	13.560	3433382	530193	99.600
4	13.830	5109	1406	0.148
5	14.175	2685	617	0.078
6	14.429	1862	371	0.054
Total		3447157	533343	100.000