

Sample Name :Hexarelin
 Cat No. : RP17315
 Lot No. : E4901619I
 Time Processed :10:02:53 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

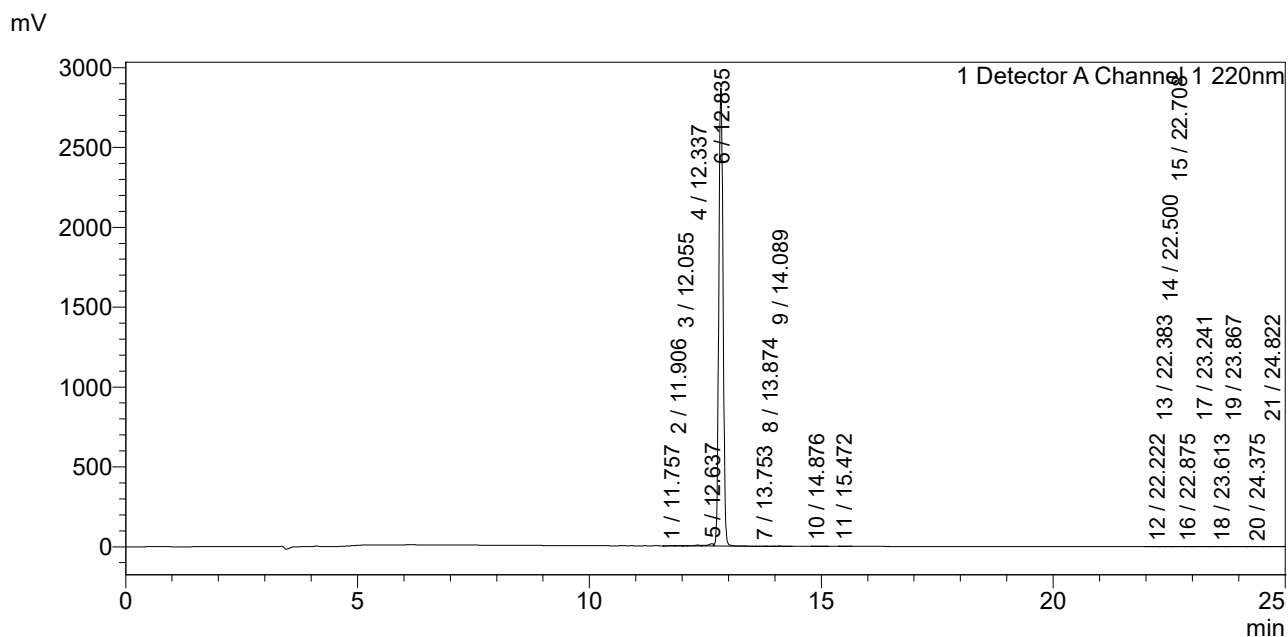

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.757	16626	2137	0.088
2	11.906	13537	1604	0.072
3	12.055	6640	1229	0.035
4	12.337	62890	5719	0.335
5	12.637	128076	14496	0.682
6	12.835	18521252	2867775	98.583
7	13.753	2741	458	0.015
8	13.874	3553	613	0.019
9	14.089	7259	946	0.039
10	14.876	2724	401	0.014
11	15.472	3400	572	0.018
12	22.222	2190	172	0.012
13	22.383	1083	136	0.006
14	22.500	1130	132	0.006
15	22.708	1525	154	0.008

Peak#	Ret. Time	Area	Height	Area%
16	22.875	1155	135	0.006
17	23.241	2745	165	0.015
18	23.613	2275	145	0.012
19	23.867	2560	157	0.014
20	24.375	1258	94	0.007
21	24.822	2913	237	0.016
Total		18787530	2897479	100.000