

Sample Name :PLP(139-151)
 Cat. No. : RP10550
 Lot. No. :PE0681805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

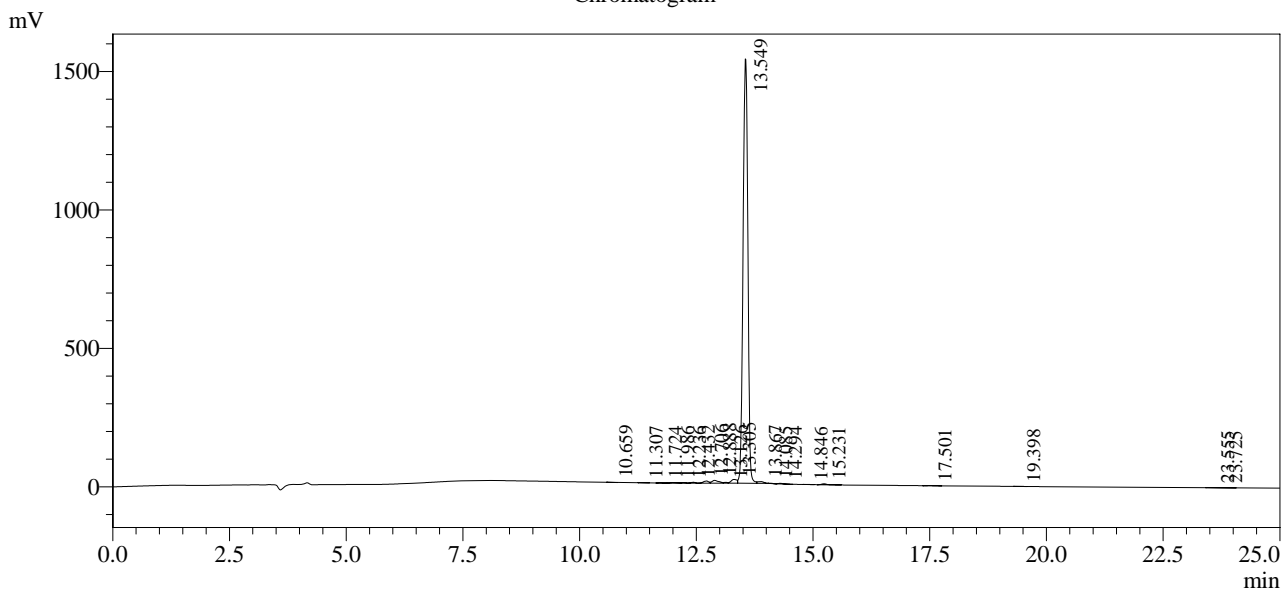

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.659	3815	576	0.033
2	11.307	1956	222	0.017
3	11.724	2188	339	0.019
4	11.986	11494	1150	0.100
5	12.236	7896	1417	0.069
6	12.432	18591	3036	0.162
7	12.706	64357	8050	0.562
8	12.888	103233	10156	0.902
9	13.126	17908	3154	0.157
10	13.305	118762	13760	1.038
11	13.549	10961265	1533043	95.795
12	13.867	57459	6215	0.502
13	14.085	5086	1011	0.044
14	14.294	18678	2421	0.163
15	14.846	2753	403	0.024
16	15.231	28979	3665	0.253
17	17.501	4773	436	0.042
18	19.398	3107	363	0.027
19	23.555	4484	458	0.039
20	23.725	5618	506	0.049
Total		11442401	1590381	100.000