

Sample Name: Bim BH3, Peptide IV Cat.
 No. : RP20339
 Lot. No. : E3393219H
 Time Processed: 11:23:17 AM
 Month-Day-Year Processed :09/05/2019
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

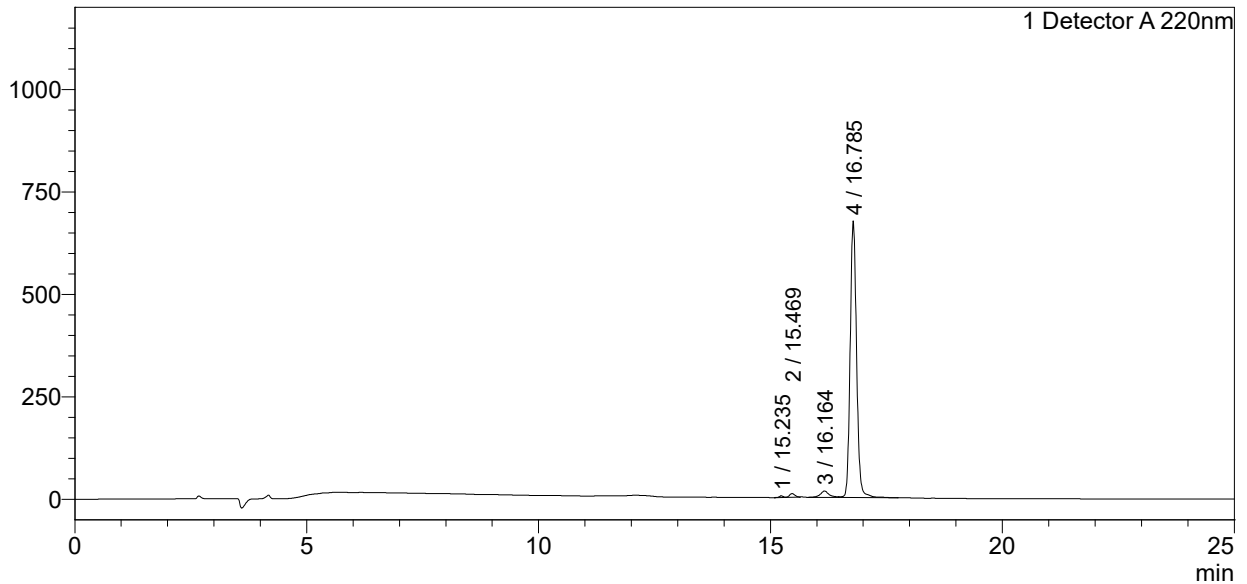

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.235	20210	3680	0.299
2	15.469	67293	8608	0.994
3	16.164	210279	15648	3.107
4	16.785	6469342	674995	95.600
Total		6767125	702931	100.000