

Sample Name : Neurotensin (8-13)  
Cat. No. : RP10442  
Lot. No. : PR1071710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

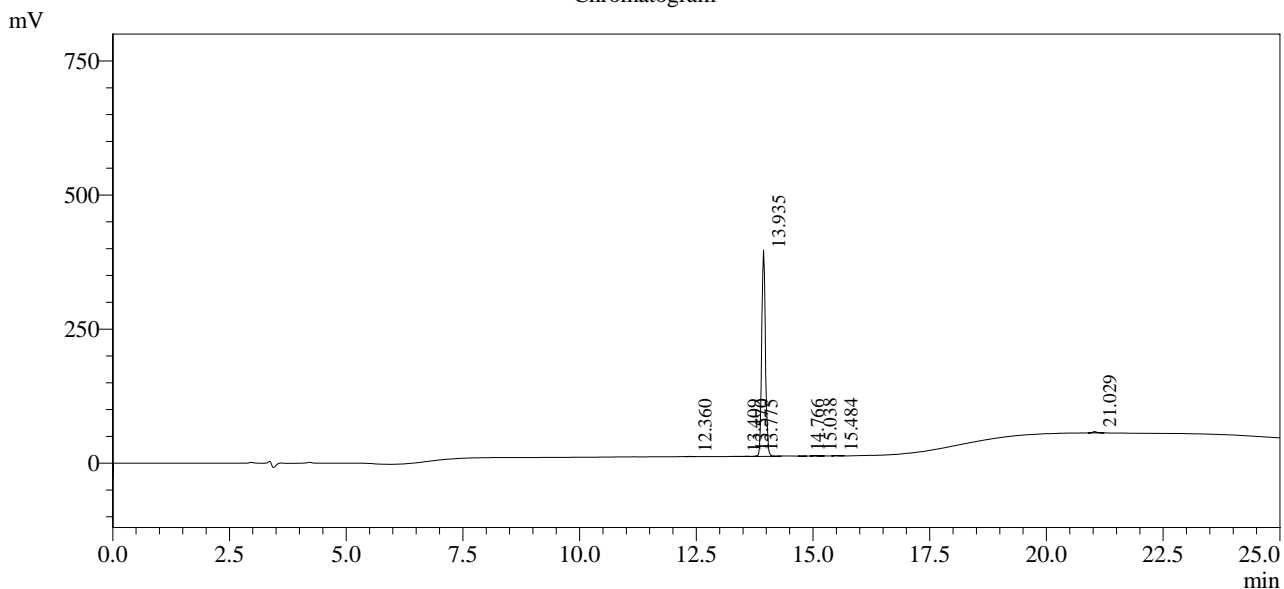

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.360	2311	407	0.105
2	13.409	608	137	0.028
3	13.570	2103	416	0.096
4	13.775	2176	831	0.099
5	13.935	2166114	384901	98.439
6	14.766	1466	285	0.067
7	15.038	5043	983	0.229
8	15.484	3881	769	0.176
9	21.029	16758	2471	0.762
Total		2200459	391199	100.000