

Sample Name :CLIP (86-100)
 Cat No.: RP20279
 Lot No.: E2732020K
 Time Processed :8:55:12
 Month-Day-Year Processed :11/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

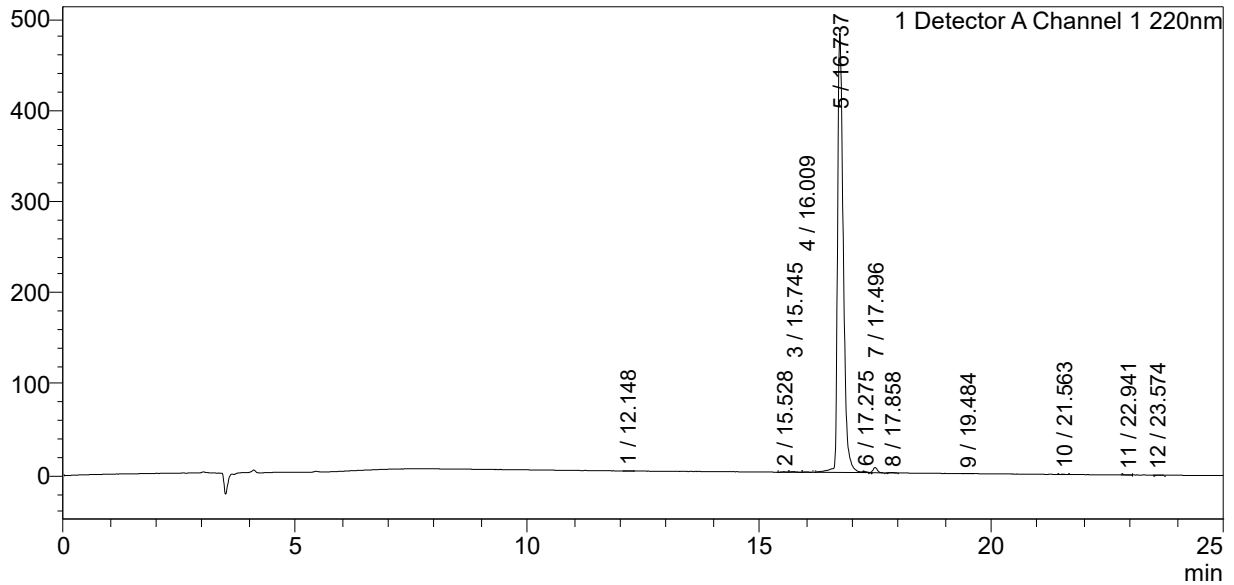

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.148	1064	129	0.026
2	15.528	3155	453	0.076
3	15.745	5086	530	0.122
4	16.009	2263	376	0.054
5	16.737	4115090	481021	98.639
6	17.275	2283	474	0.055
7	17.496	34789	5581	0.834
8	17.858	2274	310	0.055
9	19.484	1409	173	0.034
10	21.563	1050	180	0.025
11	22.941	2349	269	0.056
12	23.574	1058	154	0.025
Total		4171871	489650	100.000