

Sample Name : Hexa-His
 Cat No : RP11737
 Lot No : E7889820L
 Time Processed : 4:21:39 PM
 Month-Day-Year Processed : 12/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	10
25.00	Pumps	B.Conc	70
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	10
40.00	Pumps	B.Conc	10
45.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

mV

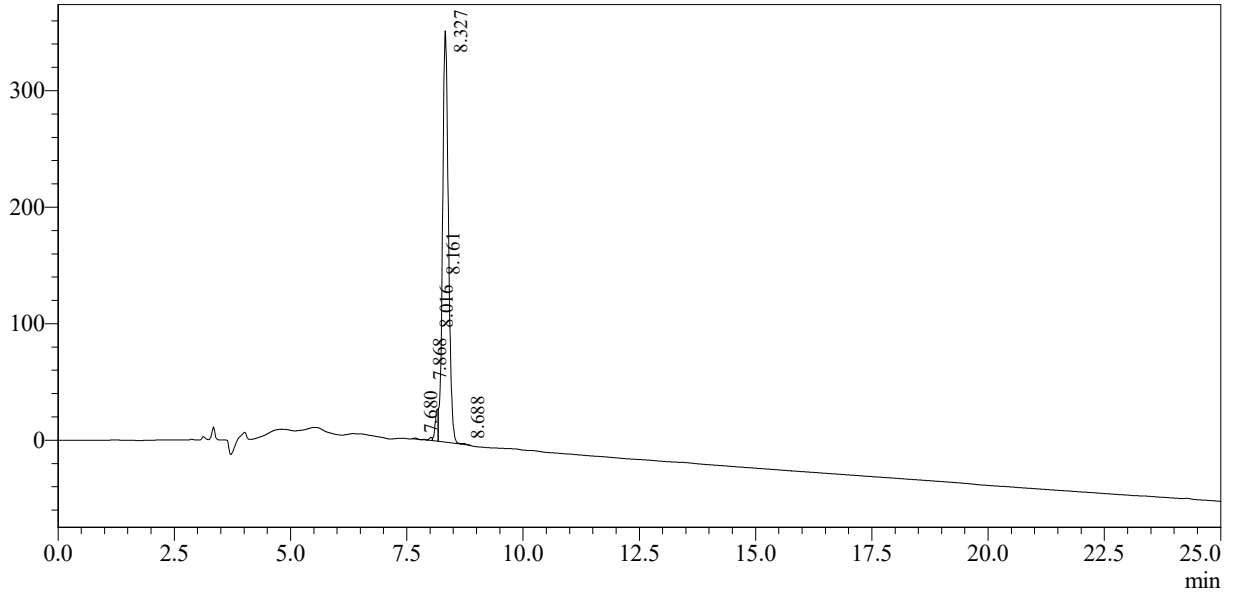

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.680	3544	778	0.109
2	7.868	1436	383	0.044
3	8.016	10626	2522	0.327
4	8.161	122301	27666	3.760
5	8.327	3109259	353073	95.580
6	8.688	5868	787	0.180
Total		3253033	385208	100.000