


# Mass Spectrum

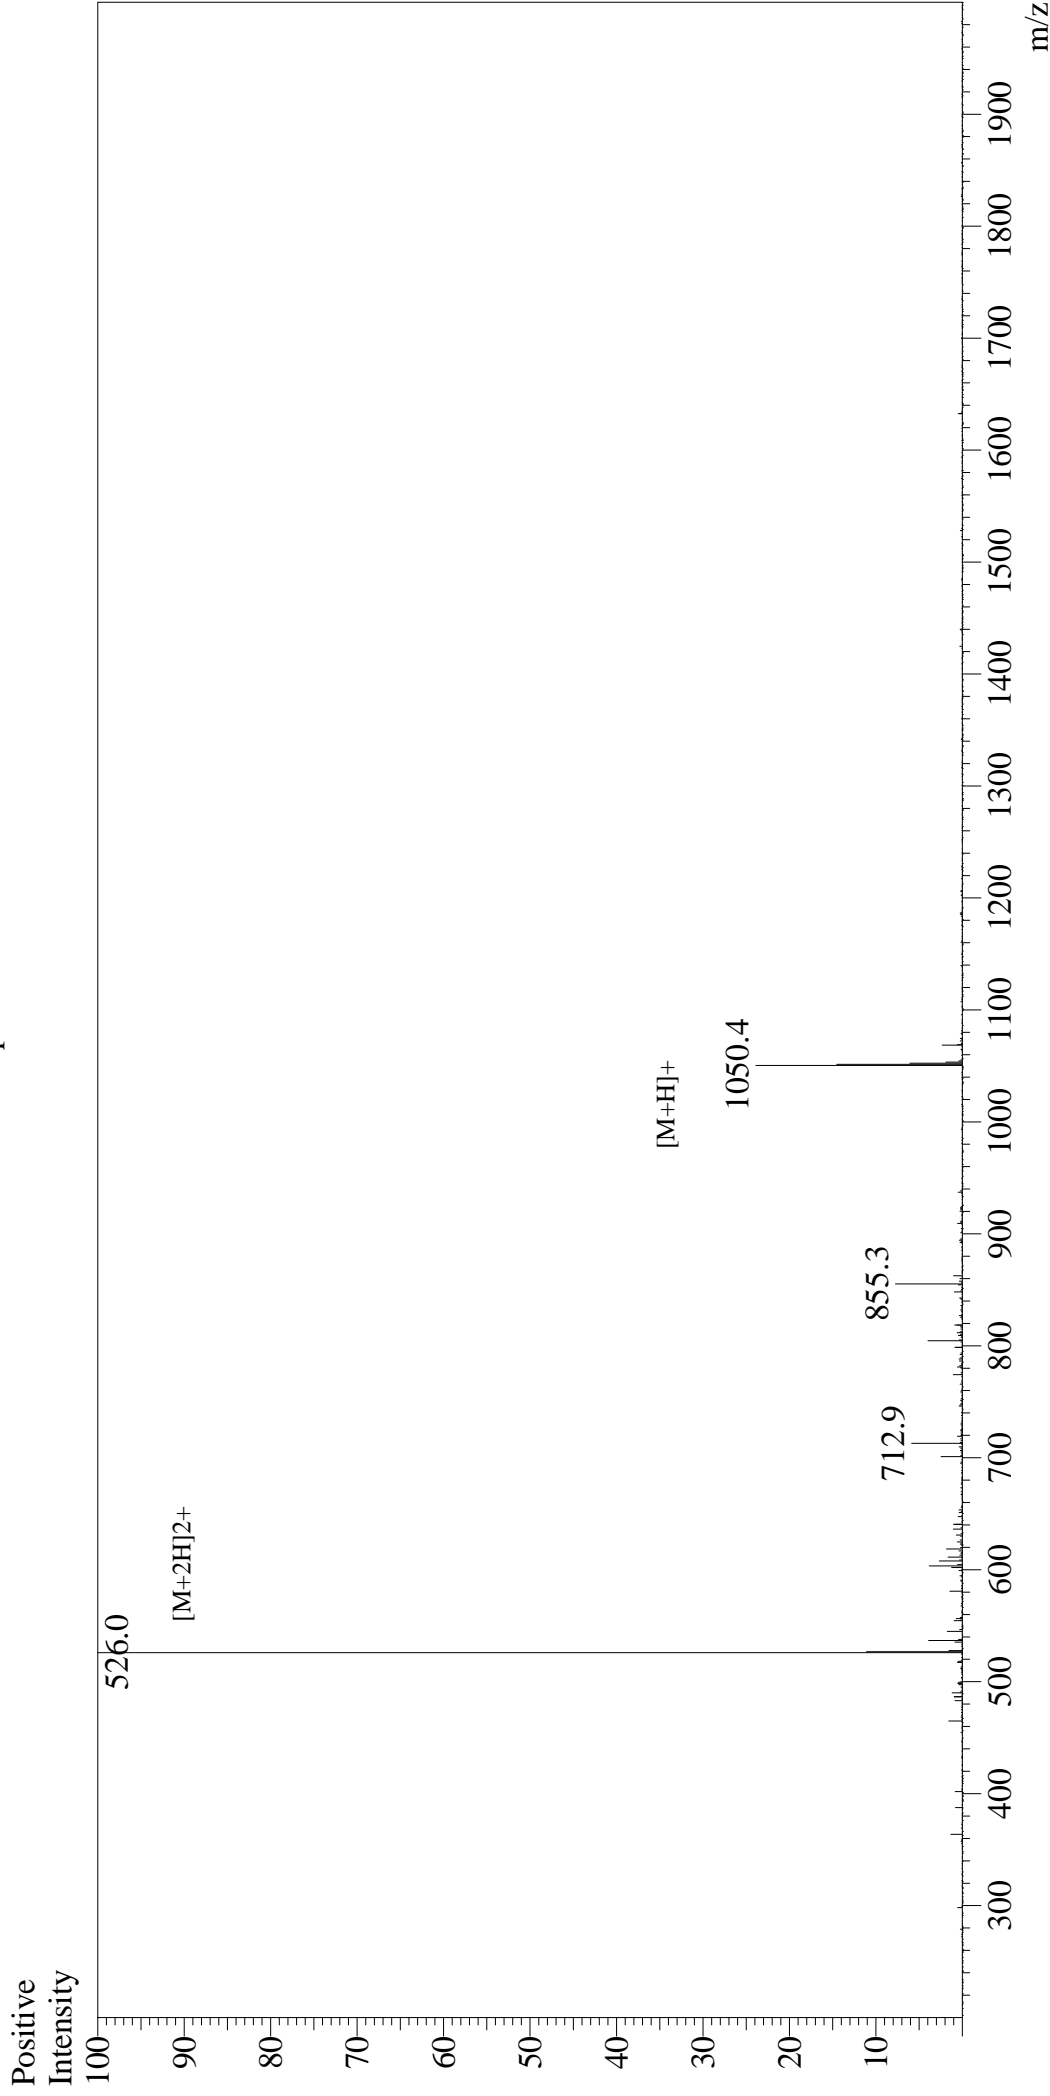

Sample Information  
User : Gary  
Month-Day Processed : 10/23/19  
Time Processed : 21:00:46  
Injection Volume : 0.3  
Sample Name : [Arg<sup>8</sup>]-Vasotocin  
Cat No. : RPI0061  
Lot No. : E1703819J  
Theoretical MW : 1050.22  
Observed MW : 1050.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH