

Sample Name :Dermorphin Analog
 Cat No. :RP13522
 Lot No. :E4911319I
 Time Processed :13:46:51
 Month-Day-Year Processed :09/22/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

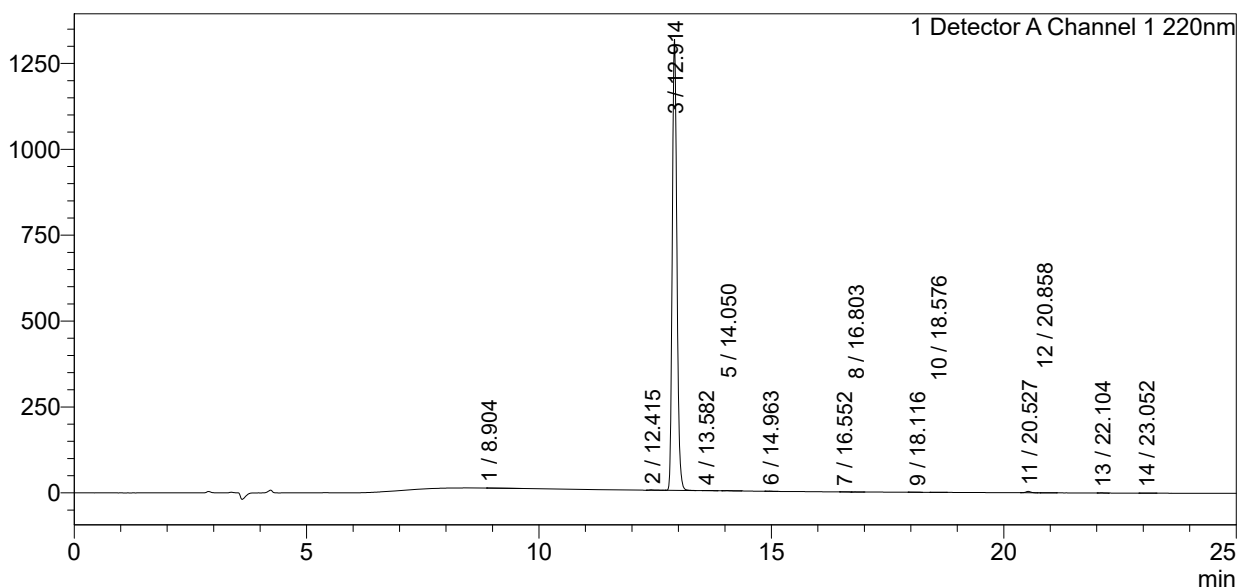

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.904	7224	81	0.079
2	12.415	9357	1162	0.102
3	12.914	9074051	1312507	99.248
4	13.582	1976	238	0.022
5	14.050	4018	498	0.044
6	14.963	3659	573	0.040
7	16.552	1511	202	0.017
8	16.803	1352	153	0.015
9	18.116	2343	292	0.026
10	18.576	2594	215	0.028
11	20.527	27901	3875	0.305
12	20.858	1970	141	0.022
13	22.104	3432	506	0.038
14	23.052	1399	166	0.015
Total		9142786	1320610	100.000