

Sample Name :Angiotensinogen (1-14), human
 Cat No. :RP10253
 Lot No. : E7155320G
 Time Processed : 7:40:50
 Month-Day-Year Processed : 07/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

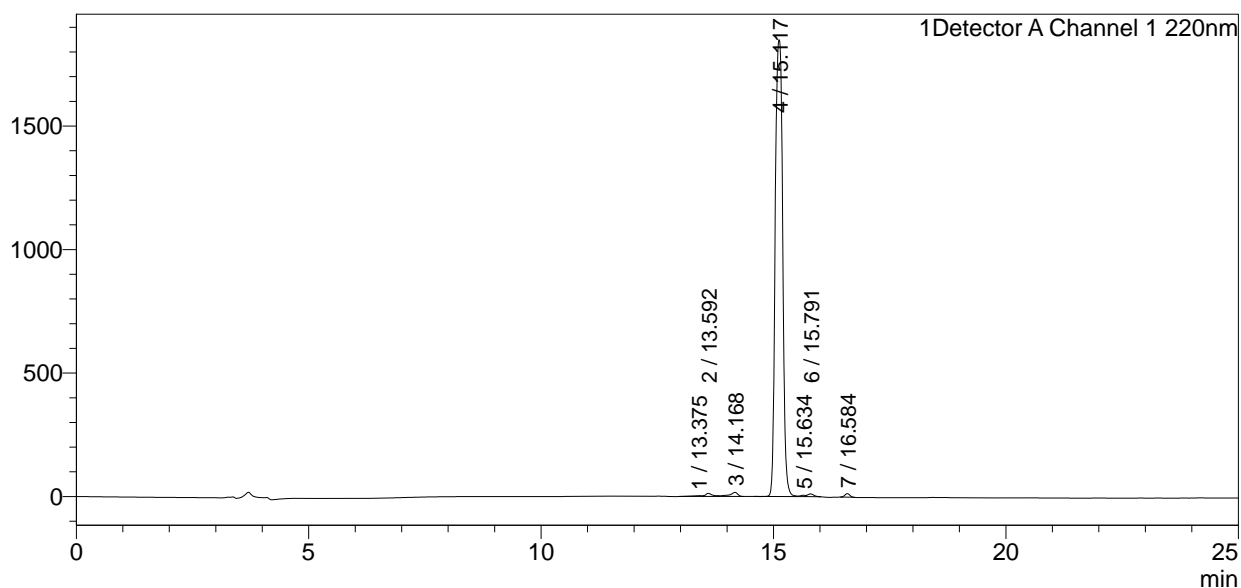

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.375	52009	3525	0.247
2	13.592	124380	12612	0.591
3	14.168	203933	16386	0.970
4	15.117	20392303	1849146	96.960
5	15.634	53864	5499	0.256
6	15.791	101105	11070	0.481
7	16.584	104083	14195	0.495
Total		21031676	1912433	100.000