

Sample Information
 Sample Name :Pancreatic Polypeptide,human
 Cat No :RP10398
 Lot No :PE7641903

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

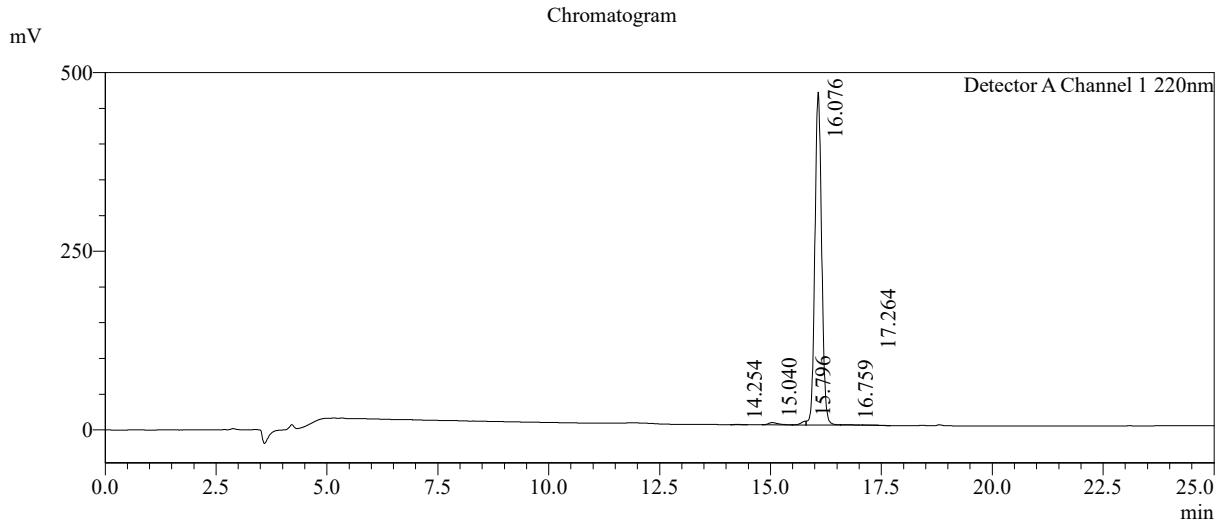

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	14.254	662	5029	0.139	0.099
2	15.040	3184	50431	0.669	0.992
3	15.796	5288	41260	1.111	0.812
4	16.076	465679	4969281	97.886	97.788
5	16.759	587	9081	0.123	0.179
6	17.264	337	6605	0.071	0.130
Total		475738	5081685	100.000	100.000